

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE121518\
 Data File : BE098495.D
 Acq On : 16 Dec 2018 6:45
 Operator : SJ/JU
 Sample : J6398-12
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C-MW-05-121118

Quant Time: Dec 17 02:55:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE121018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 10 14:59:55 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.86	152	697	0.40	ng	0.00
7) Naphthalene-d8	10.67	136	2971	0.40	ng	0.00
13) Acenaphthene-d10	14.52	164	1915	0.40	ng	-0.01
19) Phenanthrene-d10	17.27	188	5071	0.40	ng	-0.01
27) Chrysene-d12	21.46	240	6093	0.40	ng	0.00
34) Perylene-d12	24.00	264	5839	0.40	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.45	112	343	0.21	ng	0.00
5) Phenol-d6	7.04	99	290	0.13	ng	0.00
8) Nitrobenzene-d5	9.03	82	1050	0.39	ng	0.01
11) 2-Methylnaphthalene-d10	12.25	152	2107	0.44	ng	-0.01
14) 2,4,6-Tribromophenol	16.02	330	355	0.50	ng	0.00
15) 2-Fluorobiphenyl	13.15	172	3805	0.47	ng	0.00
25) Fluoranthene-d10	19.30	212	32372	0.50	ng	0.00
29) Terphenyl-d14	19.89	244	7389	0.50	ng	-0.01
Target Compounds						Qvalue
32) Bis(2-ethylhexyl)phthalate	21.35	149	2606	0.074	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE121518\
Data File : BE098495.D
Acq On : 16 Dec 2018 6:45
Operator : SJ/JU
Sample : J6398-12
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C-MW-05-121118

Quant Time: Dec 17 02:55:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE121018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 10 14:59:55 2018
Response via : Initial Calibration

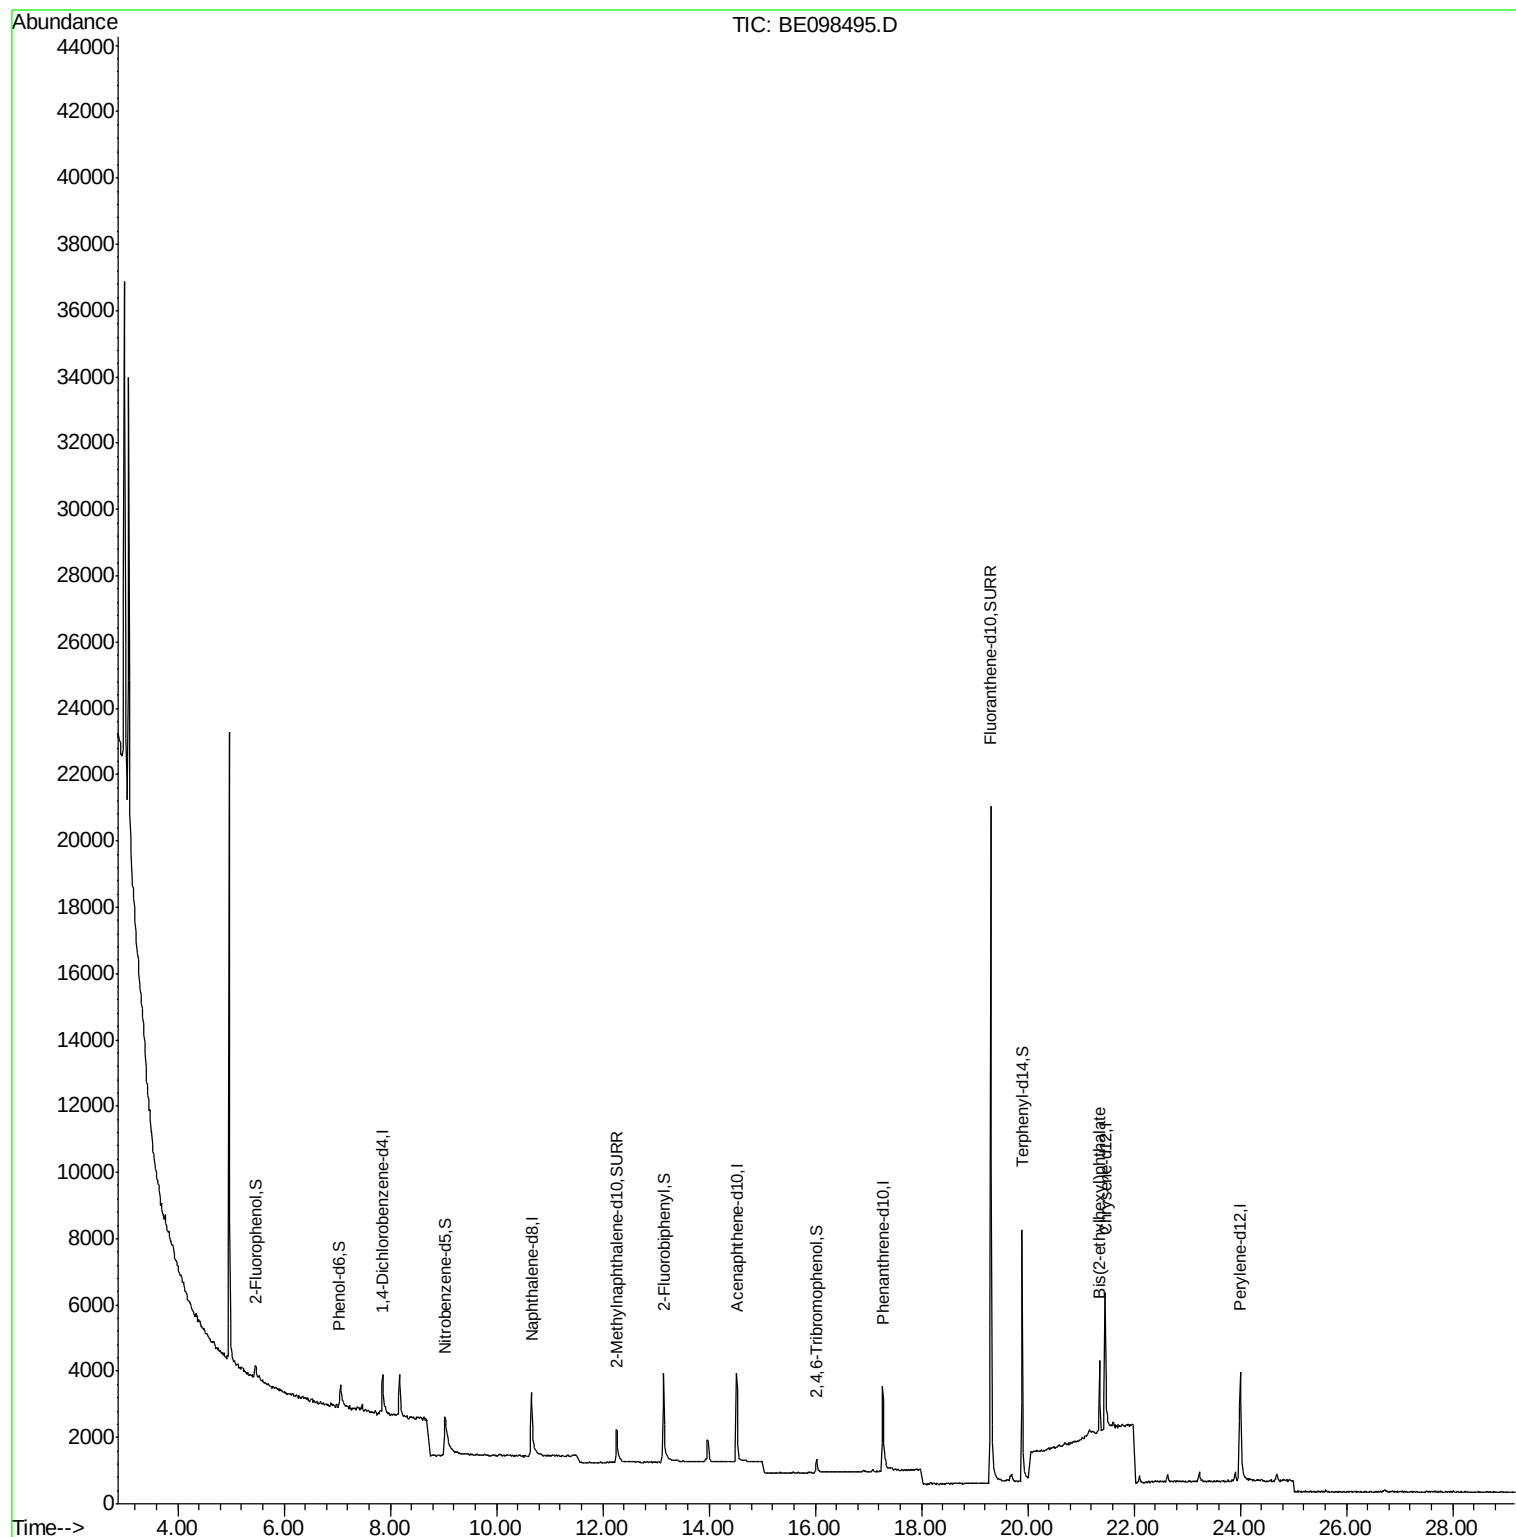

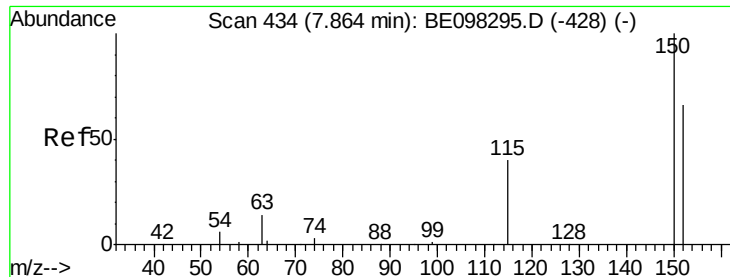


#1




1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.86 min Scan# 434
 Delta R.T. -0.00 min
 Lab File: BE098495.D
 Acq: 16 Dec 2018 6:45

Instrument :
 BNA_E
 ClientSampleId :
 C-MW-05-121118

Tot Ion	Ratio	Lower	Upper
152	100		
150	150.3	124.2	186.4
115	69.5	53.9	80.9

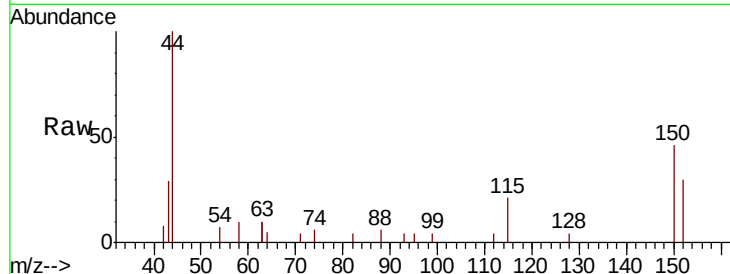


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

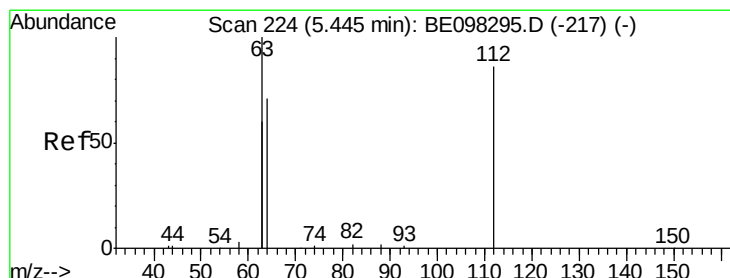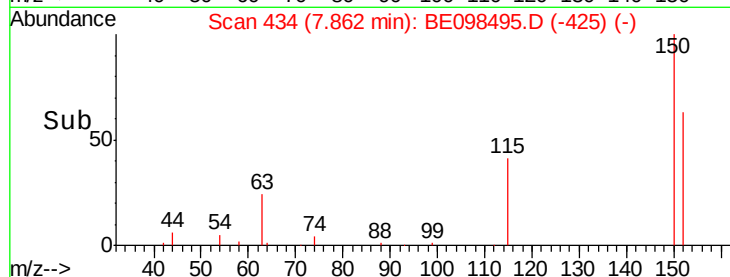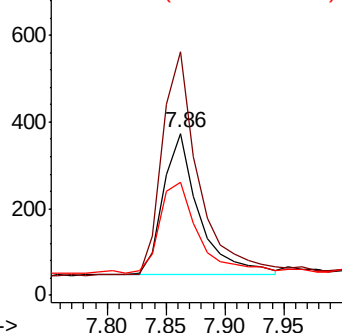



#4


2-Fluorophenol
 Concen: 0.210 ng
 RT: 5.45 min Scan# 225
 Delta R.T. 0.01 min
 Lab File: BE098495.D
 Acq: 16 Dec 2018 6:45

Tgt Ion	Ratio	Lower	Upper
112	100		
64	79.3	59.8	89.8
63	197.1	133.7	200.5

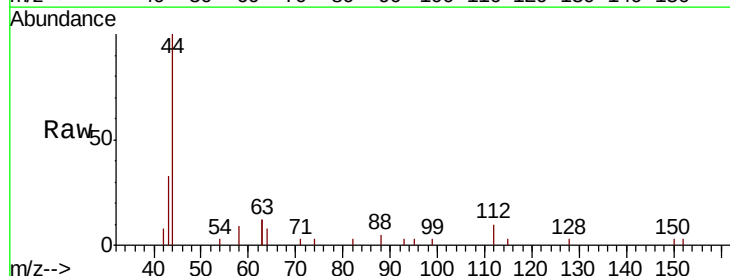

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BE0
 Ion 63.00 (62.70 to 63.70): BE0

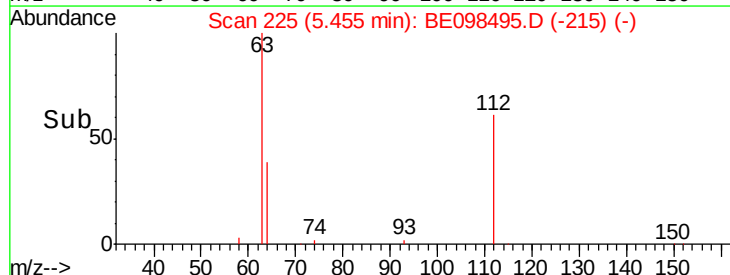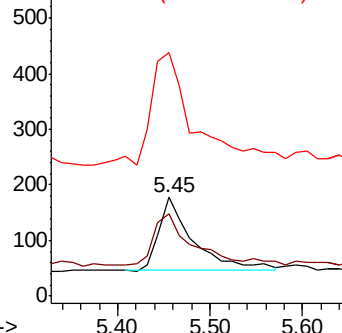

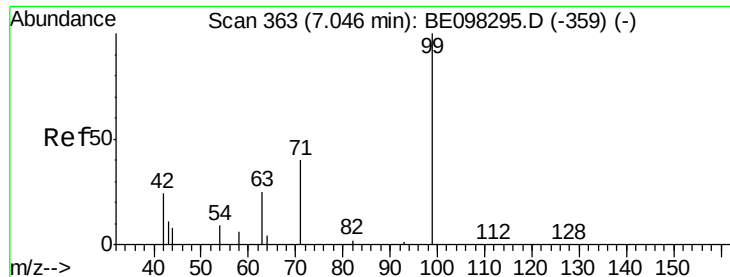

#5

Phenol-d6

Concen: 0.126 ng

RT: 7.04 min Scan# 363

Delta R.T. -0.00 min

Lab File: BE098495.D

Acq: 16 Dec 2018 6:45

Instrument :

BNA_E

ClientSampleId :

C-MW-05-121118


Tot Ion: 99 Resp: 290

Ion Ratio Lower Upper

99 100

42 56.9 26.3 39.5#




71 52.1 33.6 50.4#

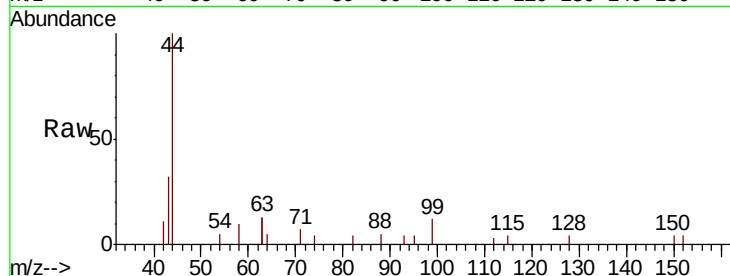

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

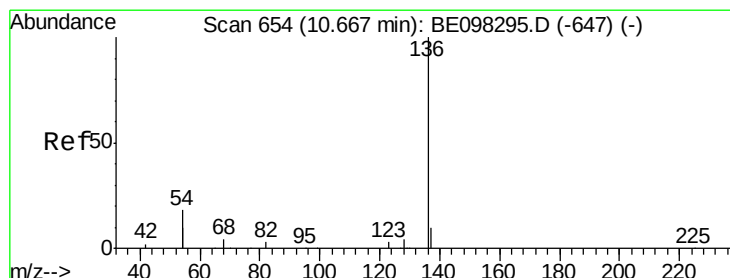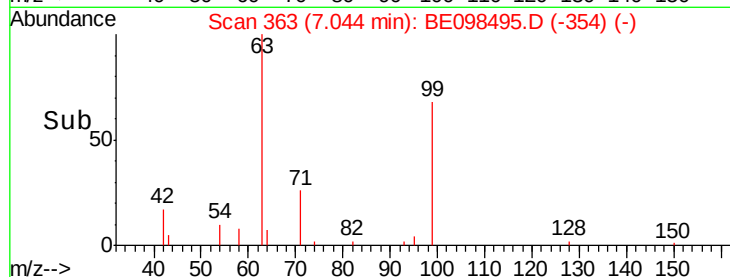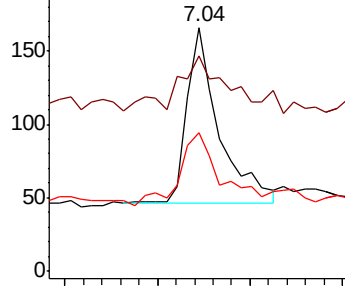

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.67 min Scan# 654

Delta R.T. -0.00 min

Lab File: BE098495.D

Acq: 16 Dec 2018 6:45

Tgt Ion: 136 Resp: 2971


Ion Ratio Lower Upper

136 100

137 14.3 9.2 13.8#

54 48.3 28.4 42.6#

68 8.9 5.4 8.0#


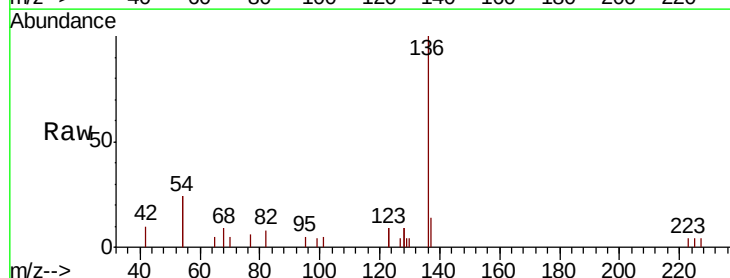



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0



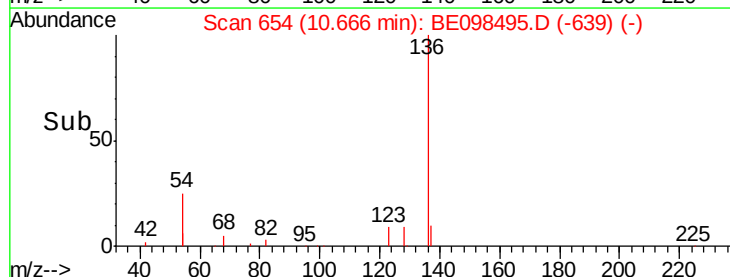
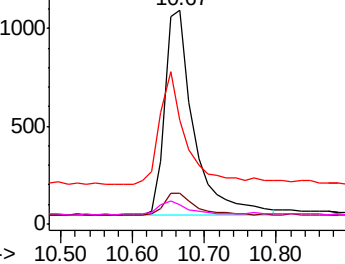


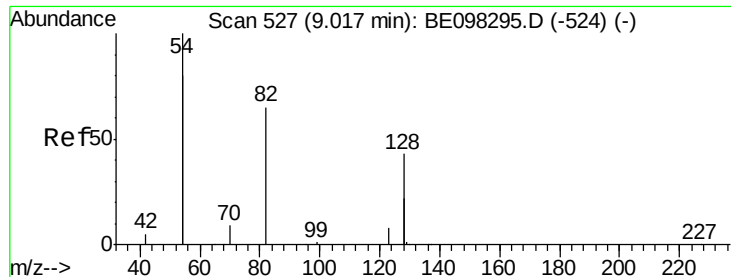

#8
 Nitrobenzene-d5
 Concen: 0.388 ng
 RT: 9.03 min Scan# 528
 Delta R.T. 0.01 min
 Lab File: BE098495.D
 Acq: 16 Dec 2018 6:45




Instrument :
 BNA_E
 ClientSampleId :
 C-MW-05-121118


Tot Ion	Ratio	Lower	Upper
82	100		
128	155.1	102.4	153.6#
54	326.5	221.8	332.8

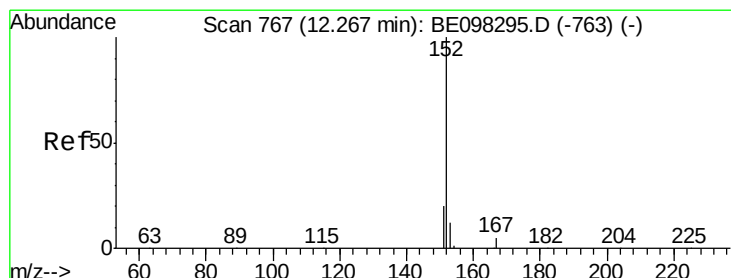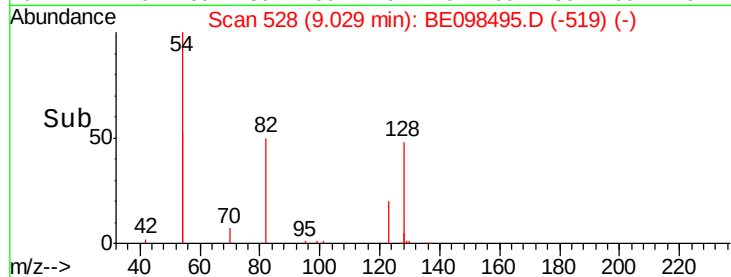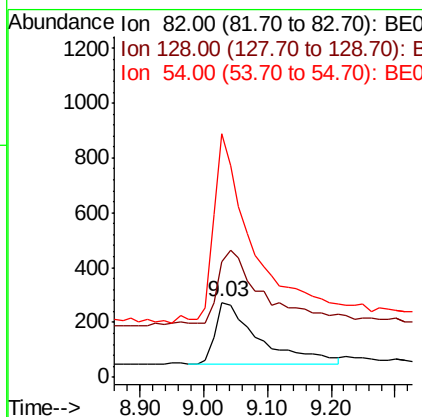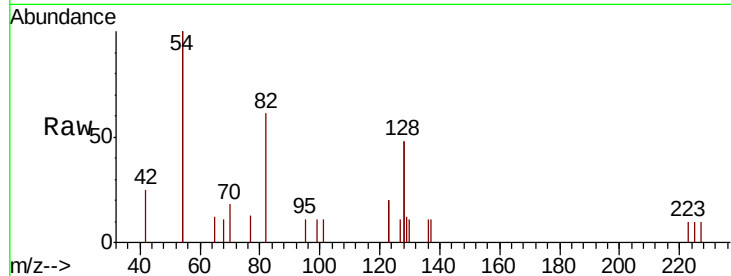

#11
 2-Methylnaphthalene-d10
 Concen: 0.436 ng
 RT: 12.25 min Scan# 766
 Delta R.T. -0.01 min
 Lab File: BE098495.D
 Acq: 16 Dec 2018 6:45

Tgt Ion	Ratio	Lower	Upper
152	100		
151	20.7	16.2	24.4


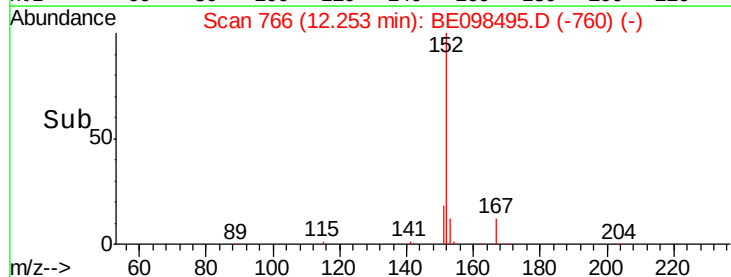
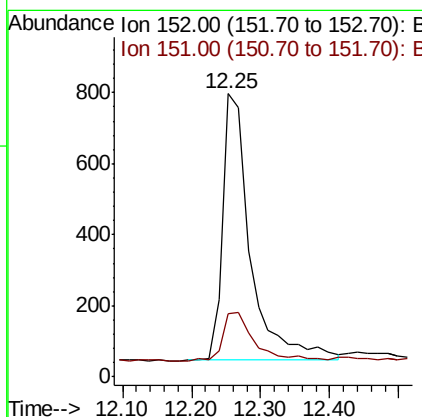
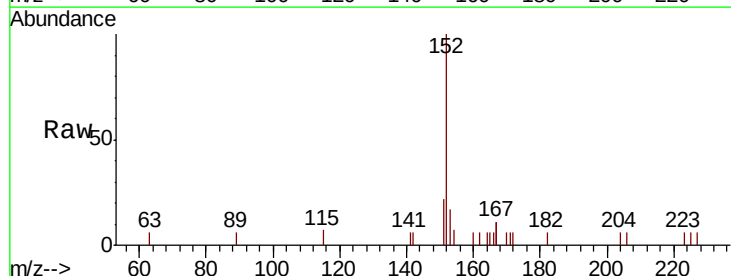


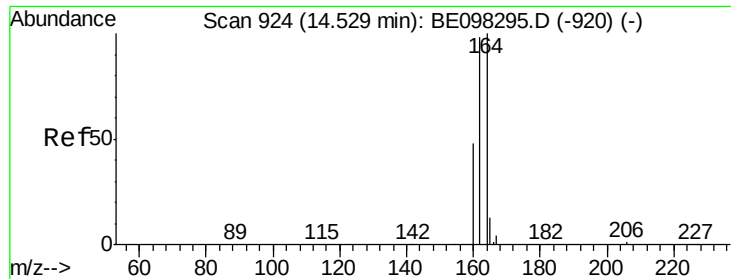

#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.52 min Scan# 923
 Delta R.T. -0.01 min
 Lab File: BE098495.D
 Acq: 16 Dec 2018 6:45




Instrument :
 BNA_E
 ClientSampleId :
 C-MW-05-121118


Tot Ion:164 Resp: 1915
 Ion Ratio Lower Upper
 164 100
 162 105.3 77.6 116.4
 160 58.9 36.0 54.0#

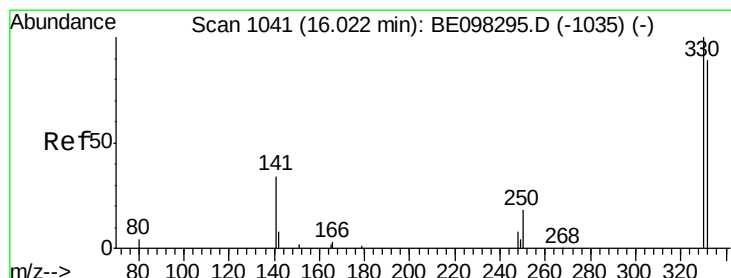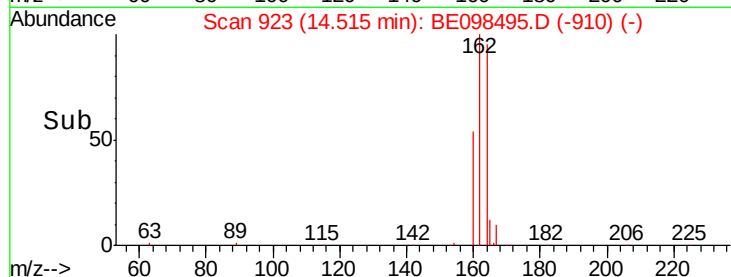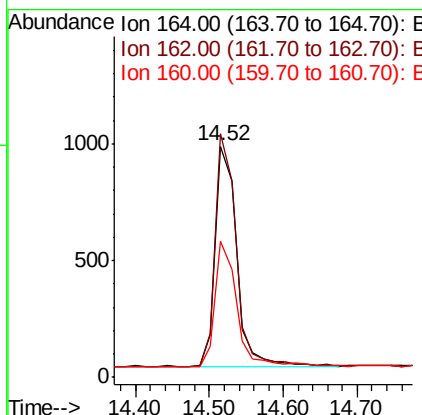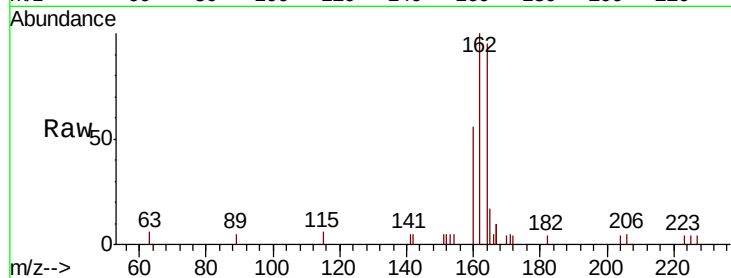

#14
 2,4,6-Tribromophenol
 Concen: 0.505 ng
 RT: 16.02 min Scan# 1041
 Delta R.T. -0.00 min
 Lab File: BE098495.D
 Acq: 16 Dec 2018 6:45

Tgt Ion:330 Resp: 355
 Ion Ratio Lower Upper
 330 100
 332 99.7 76.2 114.4
 141 46.2 39.0 58.4

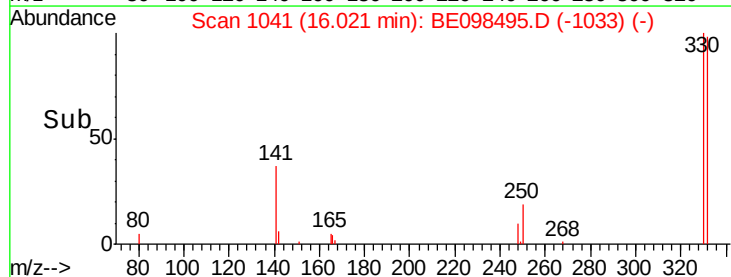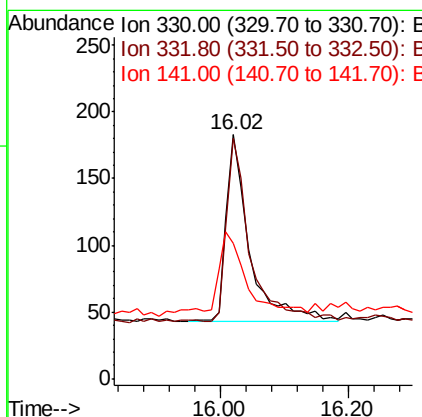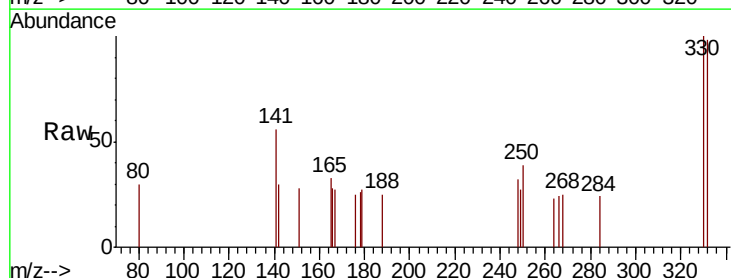

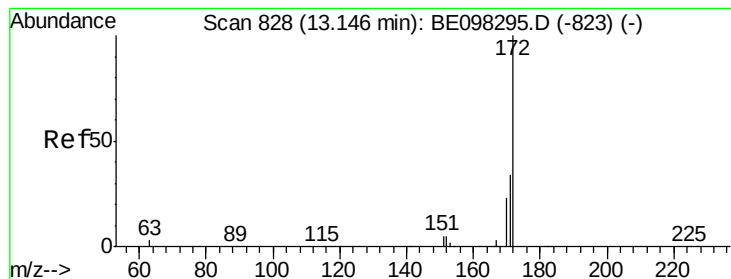

#15

2-Fluorobiphenyl

Concen: 0.471 ng

RT: 13.15 min Scan# 828

Delta R.T. 0.00 min

Lab File: BE098495.D

Acq: 16 Dec 2018 6:45

Instrument :

BNA_E

ClientSampleId :

C-MW-05-121118


Tot Ion:172 Resp: 3805

Ion Ratio Lower Upper

172 100

171 32.5 27.5 41.3




170 22.0 19.6 29.4

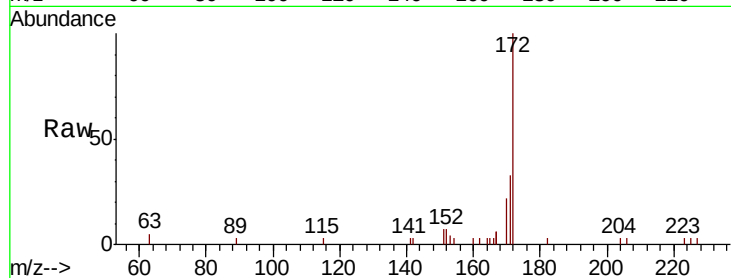

Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

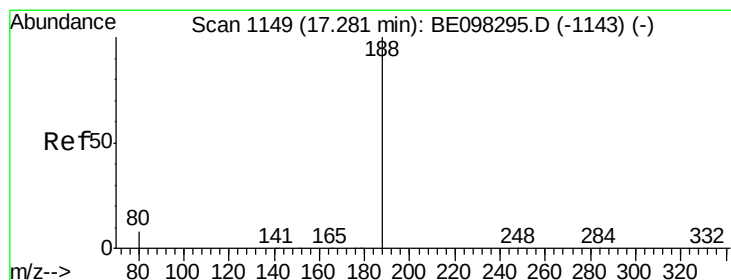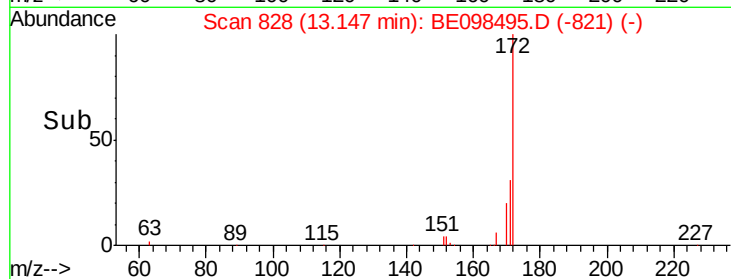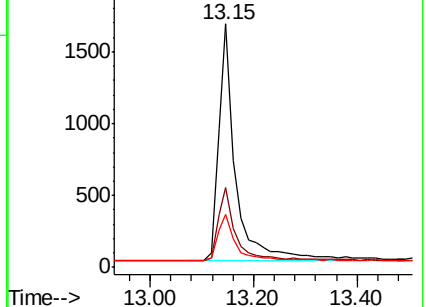

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.27 min Scan# 1148

Delta R.T. -0.01 min

Lab File: BE098495.D

Acq: 16 Dec 2018 6:45


Tgt Ion:188 Resp: 5071

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0



80 11.6 7.2 10.8#

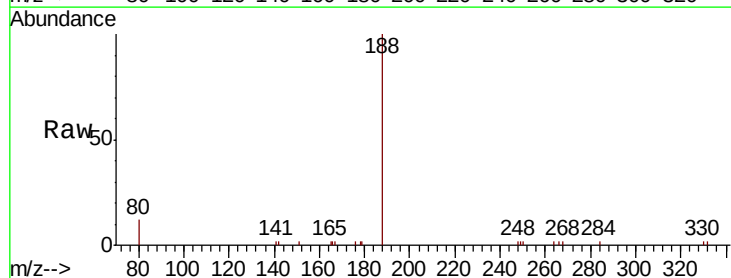


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0



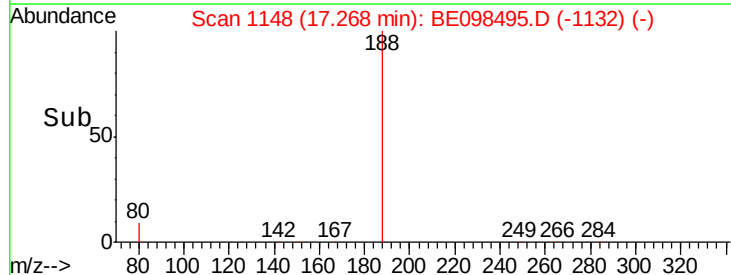
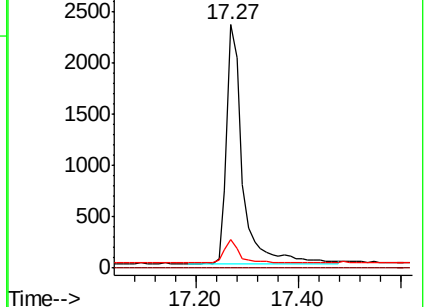


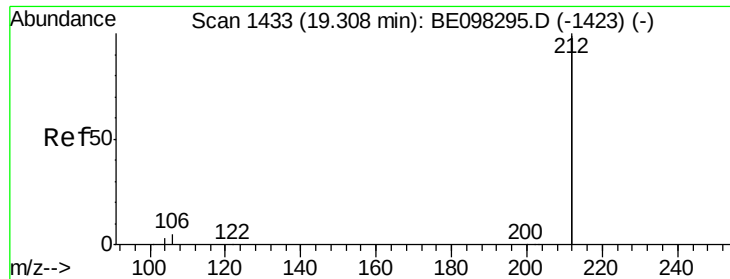

#25
Fluoranthene-d10
Concen: 0.498 ng
RT: 19.30 min Scan# 1432
Delta R.T. -0.01 min
Lab File: BE098495.D
Acq: 16 Dec 2018 6:45




Instrument :
BNA_E
ClientSampleId :
C-MW-05-121118


Tot Ion:212 Resp: 32372
Ion Ratio Lower Upper
212 100
106 2.3 2.2 3.2
104 1.3 1.3 1.9

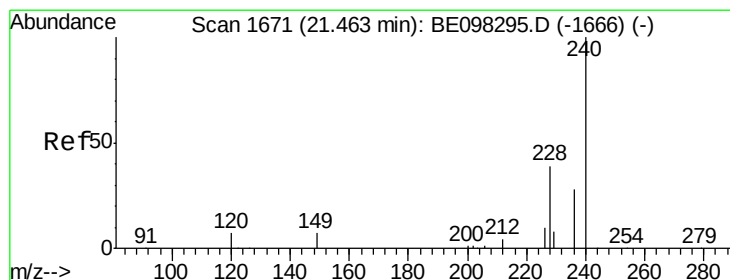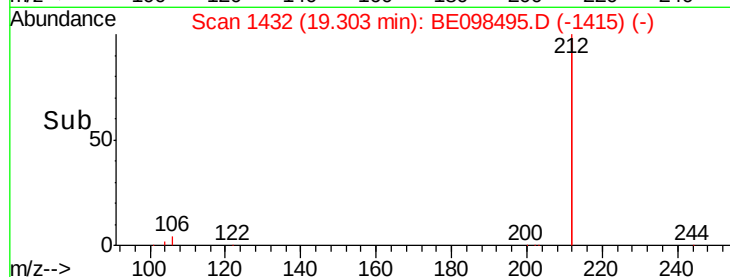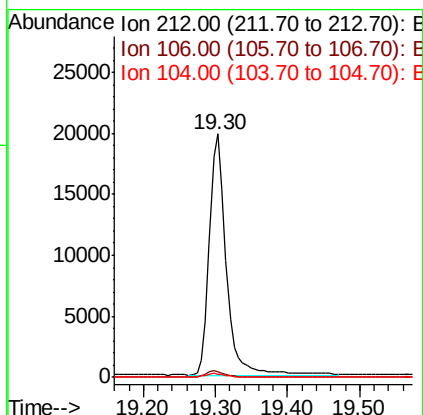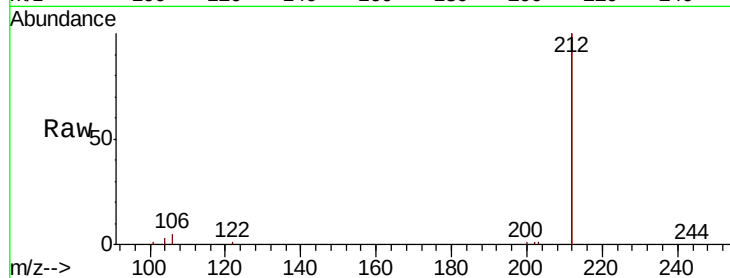

#27
Chrysene-d12
Concen: 0.400 ng
RT: 21.46 min Scan# 1671
Delta R.T. -0.00 min
Lab File: BE098495.D
Acq: 16 Dec 2018 6:45

Tgt Ion:240 Resp: 6093
Ion Ratio Lower Upper
240 100
120 7.7 9.5 14.3#
236 28.8 22.7 34.1

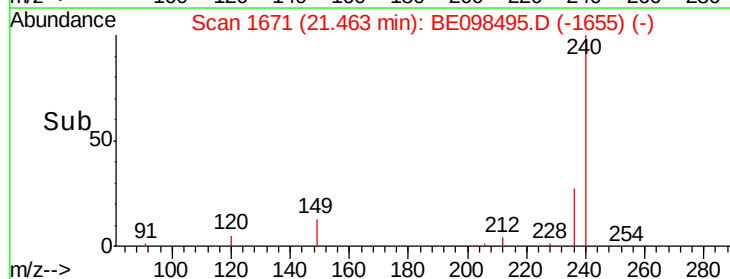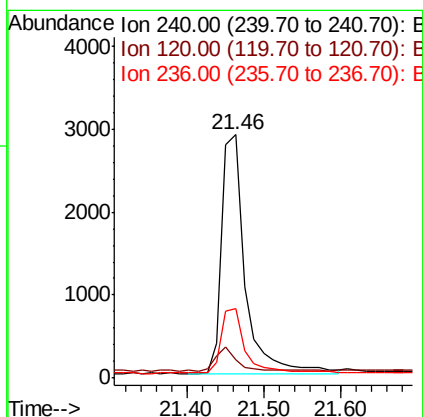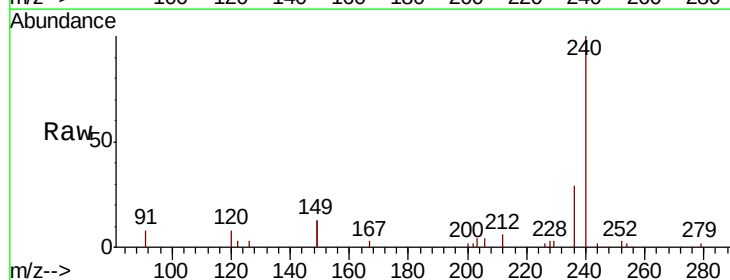

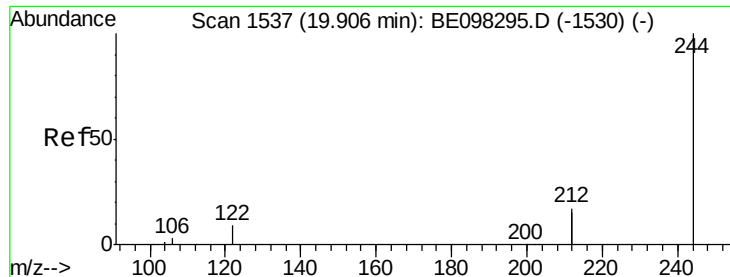

#29

Terphenyl-d14

Concen: 0.499 ng

RT: 19.89 min Scan# 1535

Delta R.T. -0.01 min

Lab File: BE098495.D

Acq: 16 Dec 2018 6:45

Instrument :

BNA_E

ClientSampleId :

C-MW-05-121118


Tot Ion:244 Resp: 7389

Ion Ratio Lower Upper




244 100

212 39.3 27.4 41.0

122 10.2 8.3 12.5

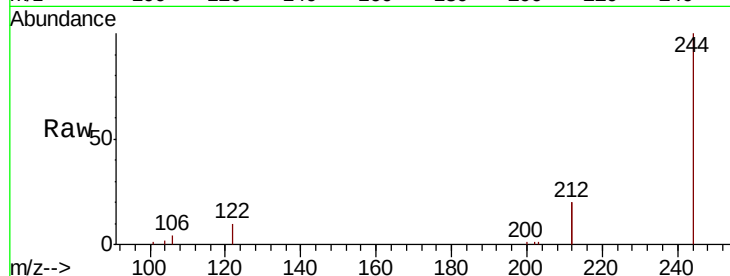

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

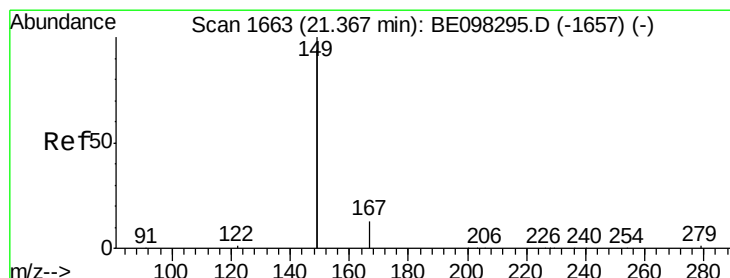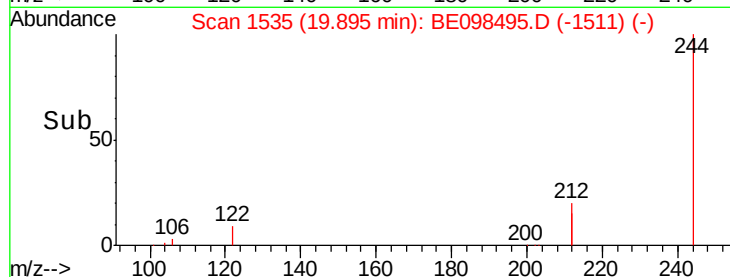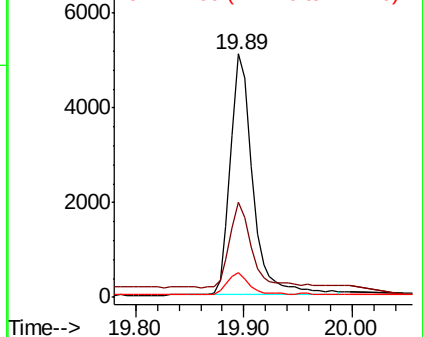

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.074 ng

RT: 21.35 min Scan# 1662

Delta R.T. -0.01 min

Lab File: BE098495.D

Acq: 16 Dec 2018 6:45


Tgt Ion:149 Resp: 2606

Ion Ratio Lower Upper



149 100




167 6.6 5.7 8.5

279 1.3 1.0 1.4

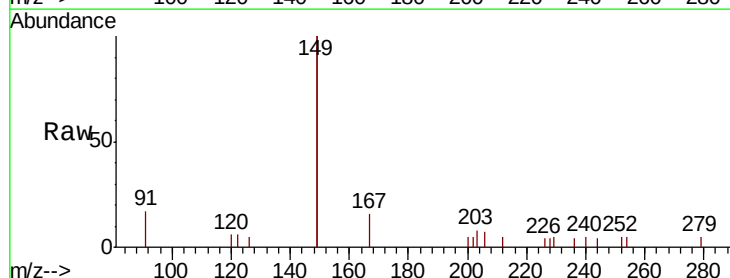

Abundance Ion 149.00 (148.70 to 149.70): E
Ion 167.00 (166.70 to 167.70): E
Ion 279.00 (278.70 to 279.70): E

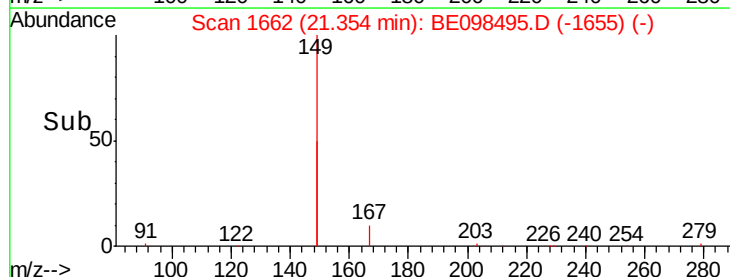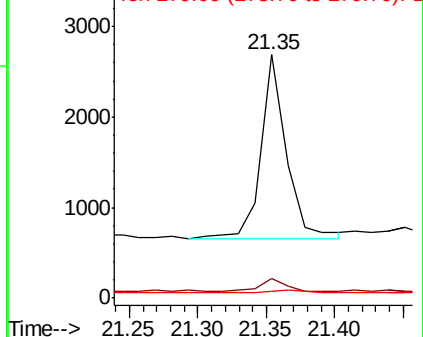

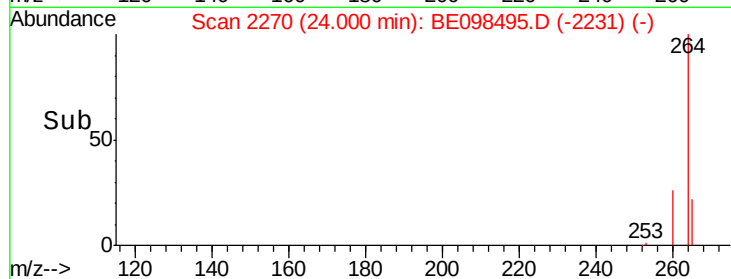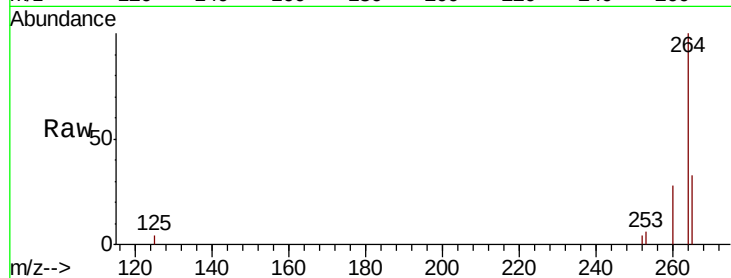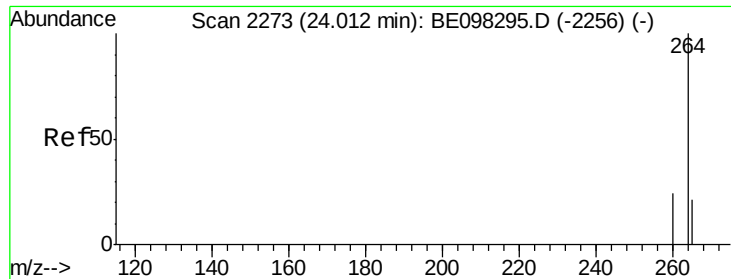

#34

Pervlene-d12

Concen: 0.400 ng

RT: 24.00 min Scan# 2270

Delta R.T. -0.01 min

Lab File: BE098495.D

Acq: 16 Dec 2018 6:45

Instrument :

BNA_E

ClientSampleId :

C-MW-05-121118

Tot Ion:264 Resp: 5839

Ion Ratio Lower Upper

264 100

260 27.6 20.2 30.2

265 32.9 25.2 37.8

