


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE121518\
 Data File : BE098486.D
 Acq On : 16 Dec 2018 00:29
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE121018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 10 14:59:55 2018

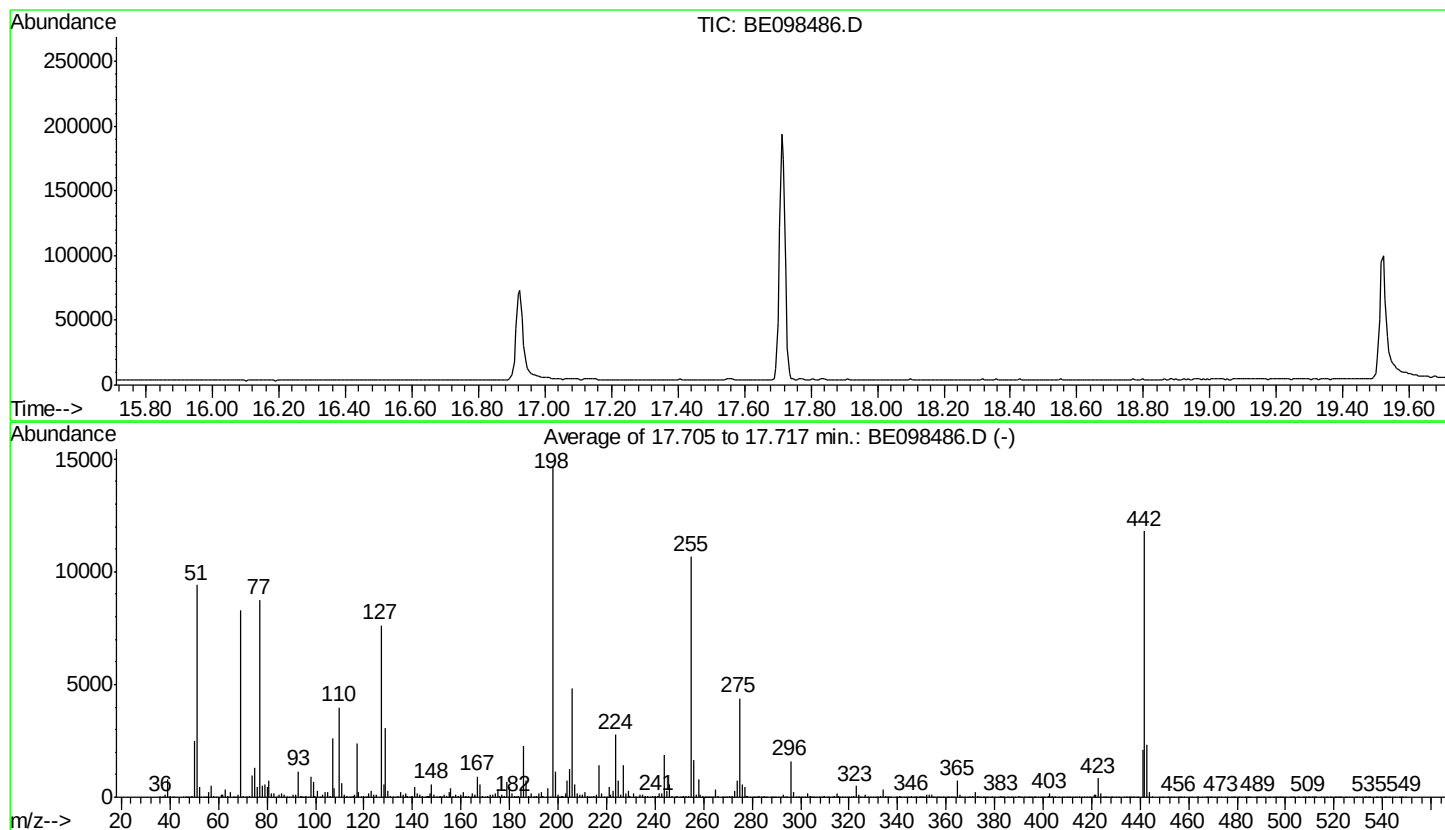

AutoFind: Scans 2573, 2574, 2575; Background Corrected with Scan 2565

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	63.9	9392	PASS
68	69	0.00	2	1.4	119	PASS
69	198	0.00	100	56.3	8275	PASS
70	69	0.00	2	0.4	37	PASS
127	198	10	80	51.9	7622	PASS
197	198	0.00	2	0.1	19	PASS
198	198	100	100	100.0	14697	PASS
199	198	5	9	7.6	1118	PASS
275	198	10	60	29.7	4372	PASS
365	198	1	100	4.9	724	PASS
441	198	0.01	100	14.4	2123	PASS
442	198	50	100	80.2	11784	PASS
443	442	15	24	20.0	2356	PASS