


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE121719\
 Data File : BE100945.D
 Acq On : 17 Dec 2019 10:21
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE120419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 13 10:42:38 2019

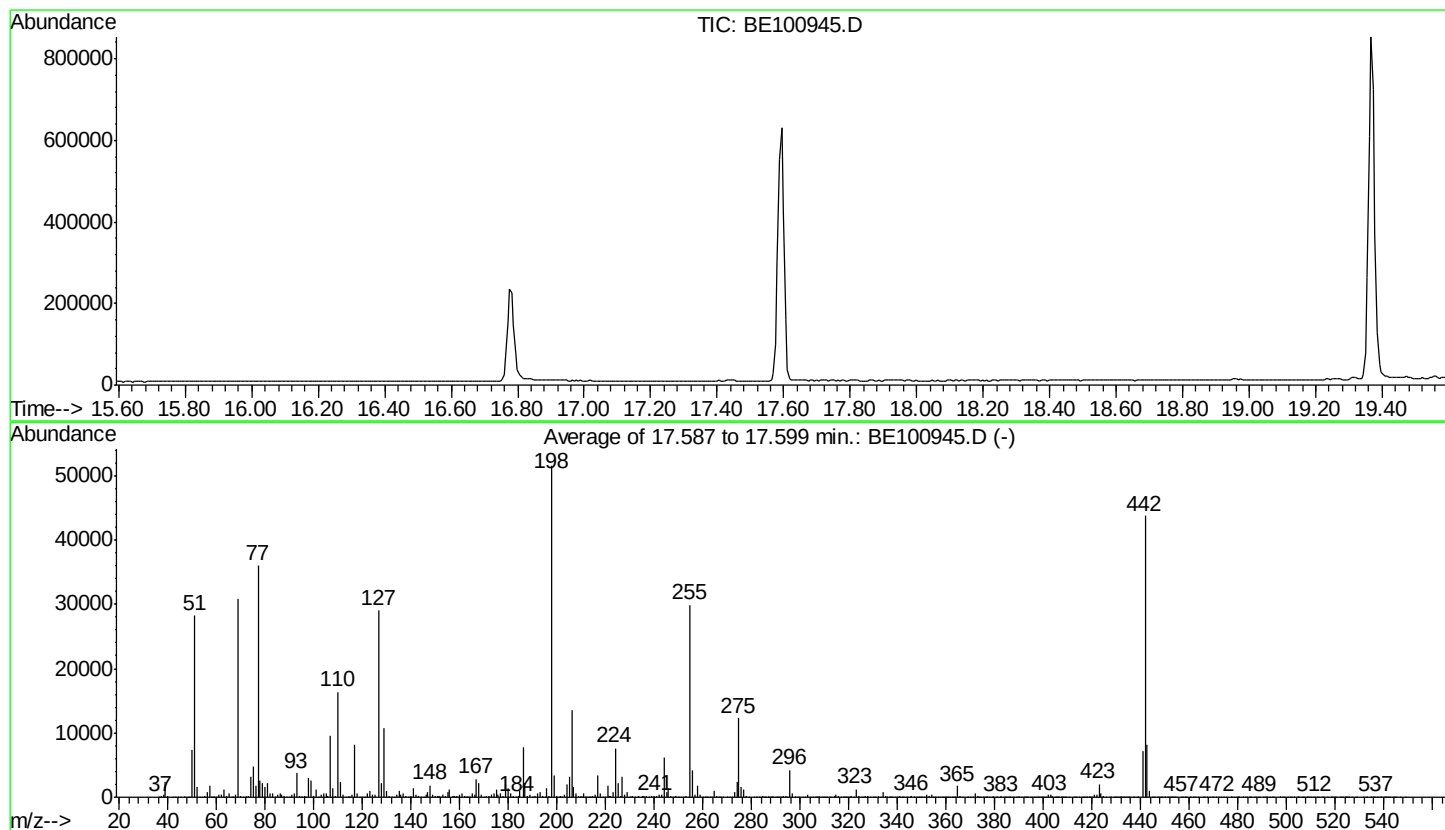

AutoFind: Scans 2553, 2554, 2555; Background Corrected with Scan 2544

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.8	28238	PASS
68	69	0.00	2	1.3	417	PASS
69	198	0.00	100	60.0	30931	PASS
70	69	0.00	2	0.5	149	PASS
127	198	10	80	56.2	28975	PASS
197	198	0.00	2	0.3	142	PASS
198	198	100	100	100.0	51555	PASS
199	198	5	9	6.6	3415	PASS
275	198	10	60	23.8	12293	PASS
365	198	1	100	3.4	1756	PASS
441	198	0.01	100	14.0	7217	PASS
442	198	50	100	84.8	43705	PASS
443	442	15	24	18.7	8174	PASS