

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE121817\
 Data File : BE095019.D
 Acq On : 18 Dec 2017 20:38
 Operator : SJ/JU
 Sample : I6900-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Quant Time: Dec 19 04:22:10 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE121817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 19 04:08:16 2017
 Response via : Initial Calibration

Instrument :
 BNA_E
 ClientSampleId :
 F9C05

Manual Integrations
 APPROVED

Sohil
 12/19/2017 4:59:37 PM

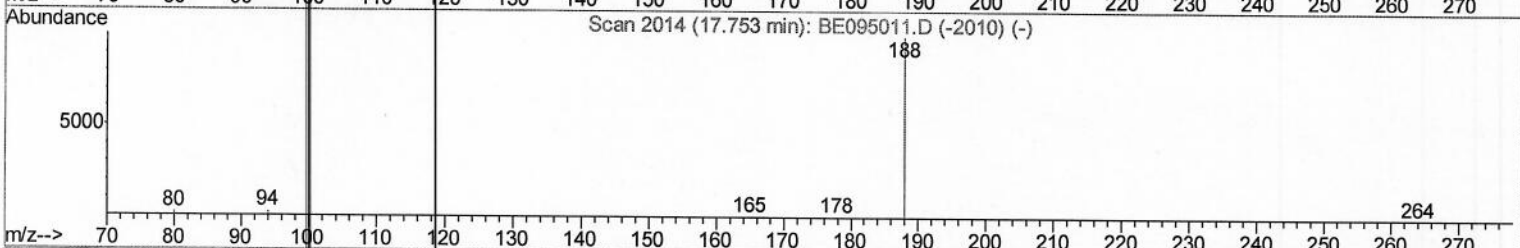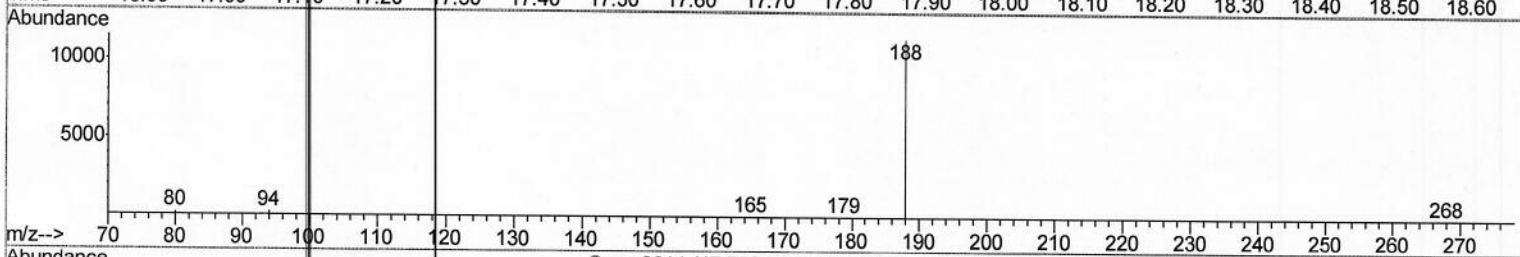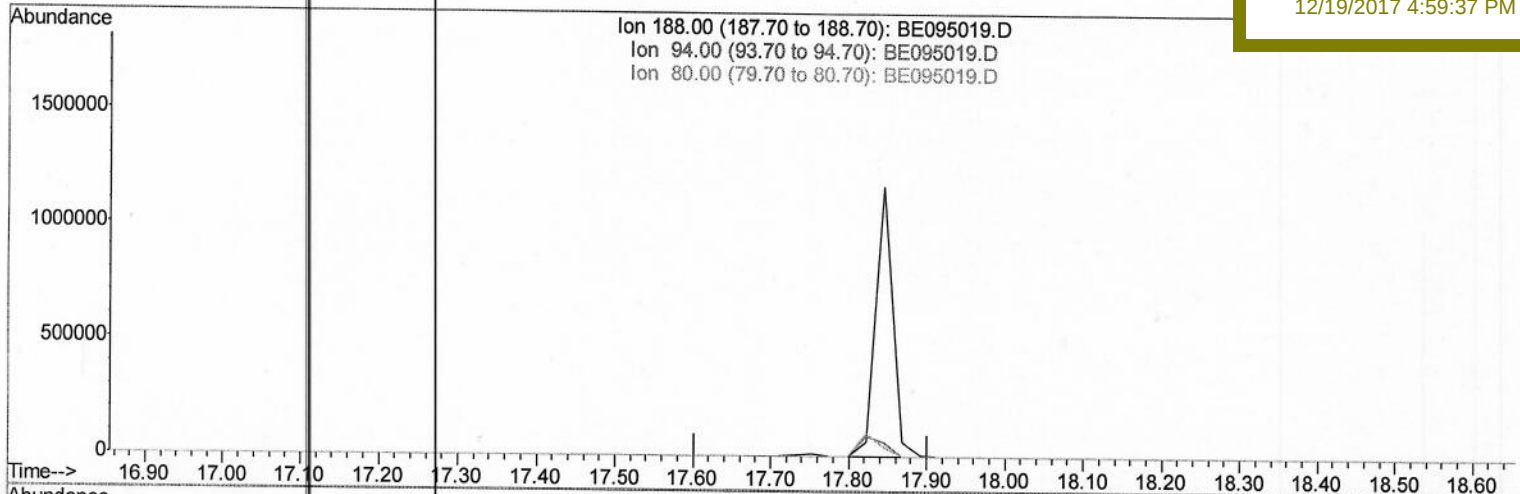

TIC: BE095019.D

(10) Phenanthrene-d10 (I)
 17.753min (-17.753) 0.00ng/ul
 response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE121817\
 Data File : BE095019.D
 Acq On : 18 Dec 2017 20:38
 Operator : SJ/JU
 Sample : I6900-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Quant Time: Dec 19 04:22:10 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE121817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 19 04:08:16 2017
 Response via : Initial Calibration

Instrument :
 BNA_E
 Client Sample Id :
 F9C05

Manual Integrations
 APPROVED

Sohil
 12/19/2017 4:59:37 PM

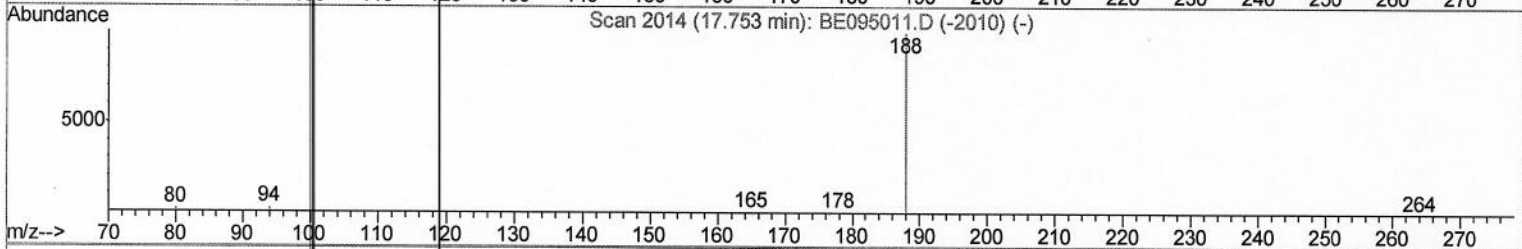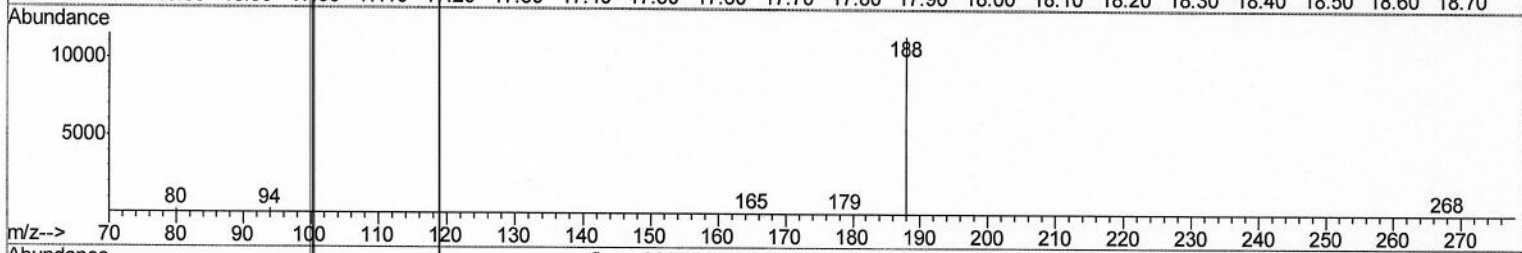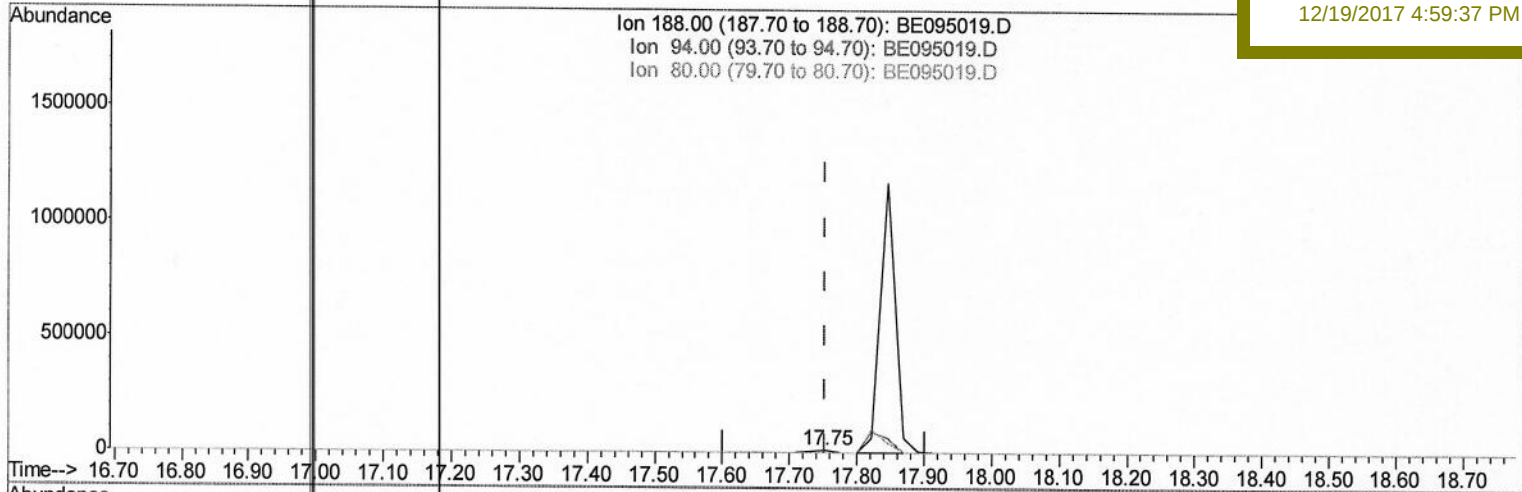

TIC: BE095019.D

(10) Phenanthrene-d10 (I)

17.753min (+0.001) 0.40ng/ul m

response 20206

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	2.29#
80.00	11.80	1.91#
0.00	0.00	0.00

SU 12/19/17

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE121817\
 Data File : BE095019.D
 Acq On : 18 Dec 2017 20:38
 Operator : SJ/JU
 Sample : I6900-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Quant Time: Dec 19 04:53:20 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE121817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 19 04:08:16 2017
 Response via : Initial Calibration

Instrument :
 BNA_E
 ClientSampleId :
 F9C05

Manual Integrations
 APPROVED

Sohil
 12/19/2017 4:59:37 PM

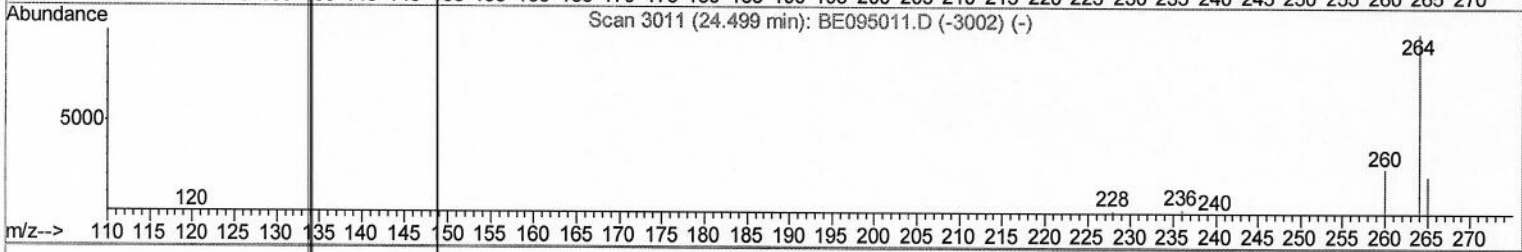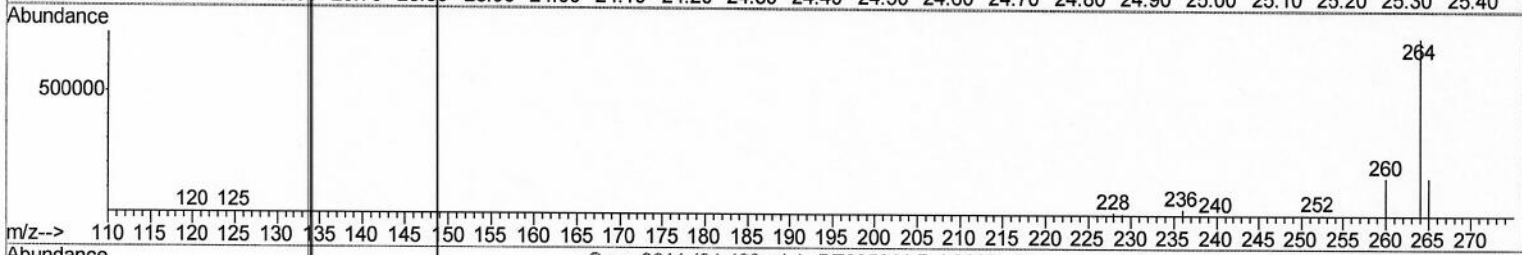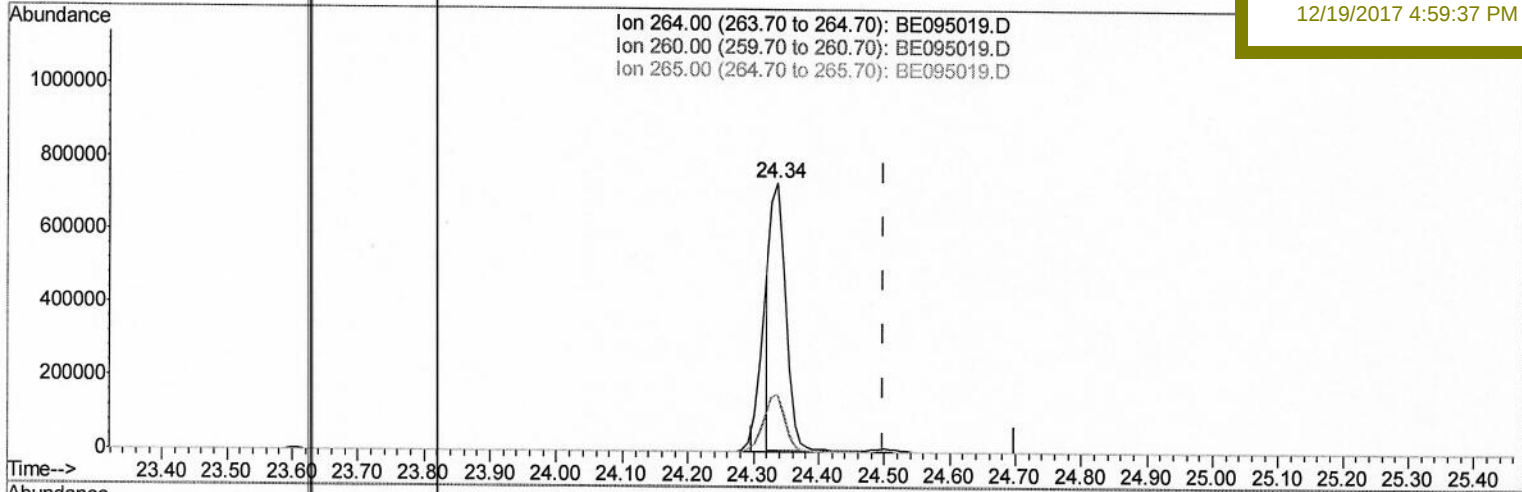

TIC: BE095019.D

(20) Perylene-d12 (I)
 24.337min (-0.162) 0.40ng/ul
 response 1216929

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.25#
265.00	103.50	21.60#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE121817\
Data File : BE095019.D
Acq On : 18 Dec 2017 20:38
Operator : SJ/JU
Sample : I6900-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Dec 19 04:53:20 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE121817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 19 04:08:16 2017
Response via : Initial Calibration

Instrument :
BNA_E
Client Sample ID :
F9C05

Manual Integrations
APPROVED

Sohil
12/19/2017 4:59:37 PM

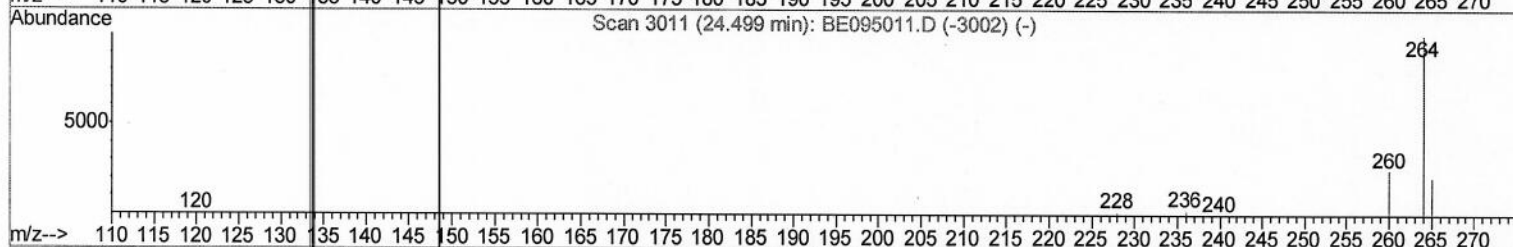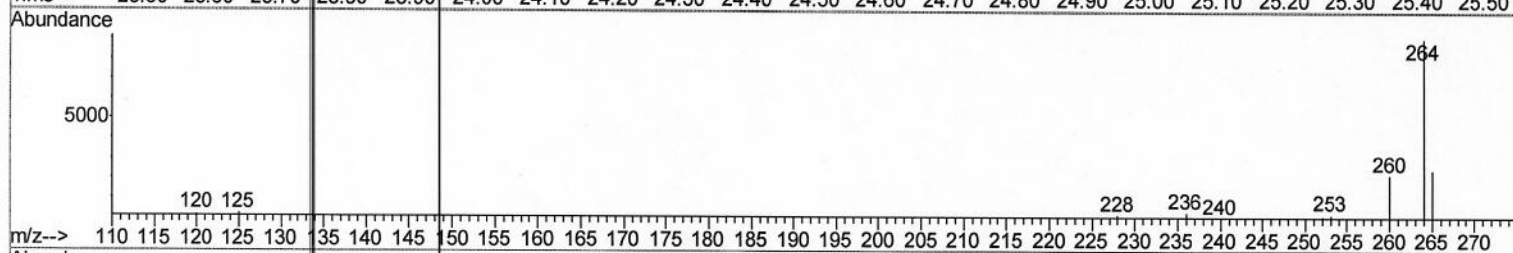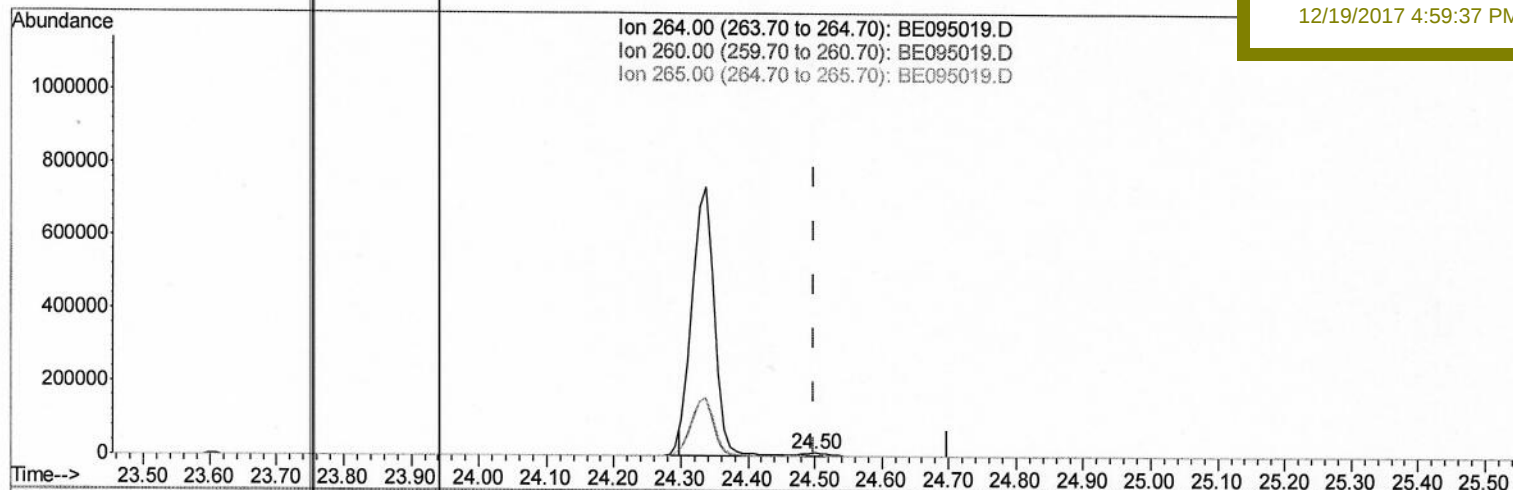

TIC: BE095019.D

(20) Perylene-d12 (I)

24.499min (+0.000) 0.40ng/ul m

response 15810

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.18
265.00	103.50	27.36#
0.00	0.00	0.00

JU 12/19/17

Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE121817\
 Data File : BE095019.D
 Acq On : 18 Dec 2017 20:38
 Operator : SJ/JU
 Sample : I6900-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Quant Time: Dec 19 04:58:39 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE121817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 19 04:08:16 2017
 Response via : Initial Calibration

Instrument :
 BNA_E
 Client Sampled :
 F9C05

Manual Integrations
 APPROVED

Sohil
 12/19/2017 4:59:37 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	8.46	152	4490	0.40	ng/ul	0.00
2) Naphthalene-d8	11.29	136	14600	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.05	164	9772	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.75	188	20206m	0.40	ng/ul	0.00
16) Chrysene-d12	21.84	240	18376	0.40	ng/ul	0.00
20) Perylene-d12	24.50	264	15810m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.85	152	8931	0.37	ng/ul	0.00
14) Fluoranthene-d10	19.72	212	23936	0.38	ng/ul	0.00
Target Compounds						
3) Naphthalene	11.34	128	1458	0.038	ng/ul#	Ovalue 81

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JU
 12/19/17

Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE121817\
 Data File : BE095019.D
 Acq On : 18 Dec 2017 20:38
 Operator : SJ/JU
 Sample : I6900-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Quant Time: Dec 19 04:58:39 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE121817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 19 04:08:16 2017
 Response via : Initial Calibration

Instrument :
 BNA_E
 ClientSampleId :
 F9C05

Manual Integrations
 APPROVED

Sohil
 12/19/2017 4:59:37 PM

