

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE121817\
 Data File : BE095022.D
 Acq On : 18 Dec 2017 22:26
 Operator : SJ/JU
 Sample : I6900-08
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F9C07

Manual Integrations
 APPROVED

Sohil
 12/19/2017 4:59:44 PM

Quant Time: Dec 19 04:22:34 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE121817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 19 04:08:16 2017
 Response via : Initial Calibration

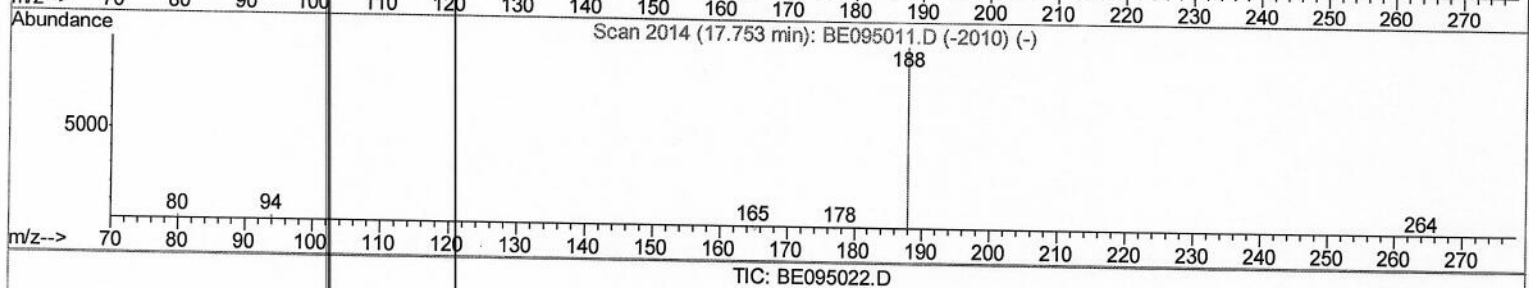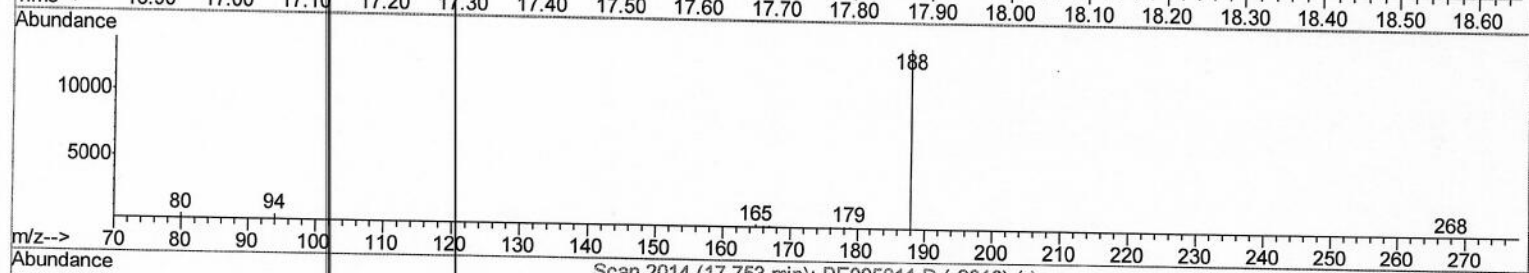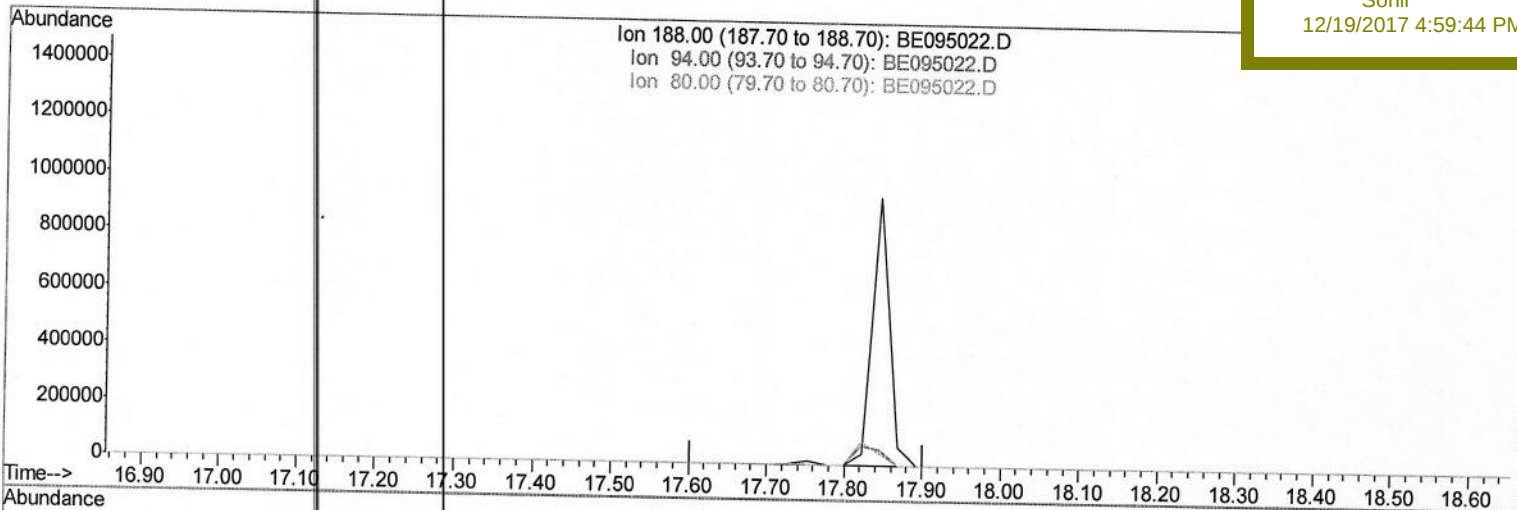

TIC: BE095022.D

(10) Phenanthrene-d10 (I)

17.753min (-17.753) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE121817\
 Data File : BE095022.D
 Acq On : 18 Dec 2017 22:26
 Operator : SJ/JU
 Sample : I6900-08
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :

BNA_E

ClientSampleId :

F9C07




Manual Integrations

APPROVED

Sohil

12/19/2017 4:59:44 PM

Quant Time: Dec 19 04:22:34 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE121817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 19 04:08:16 2017
 Response via : Initial Calibration

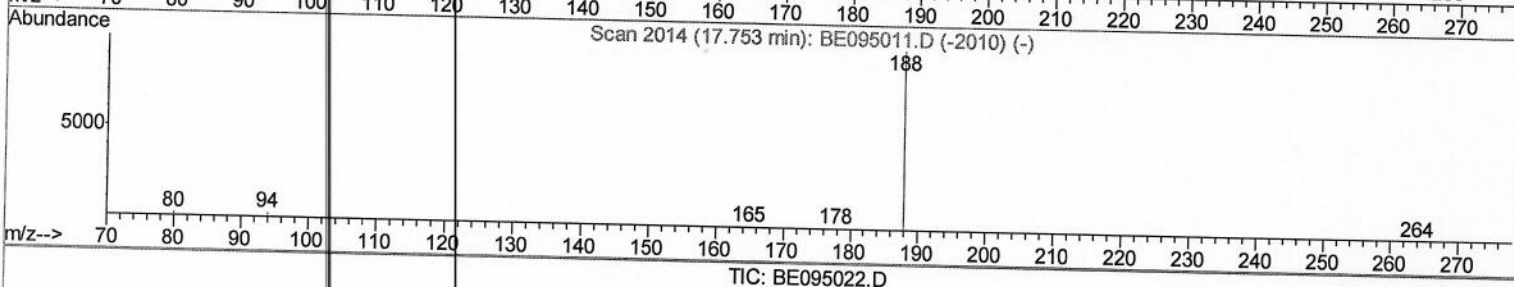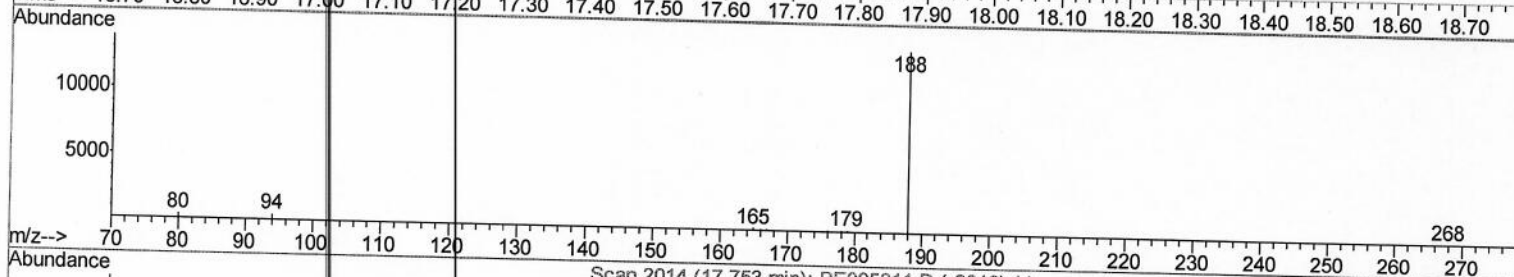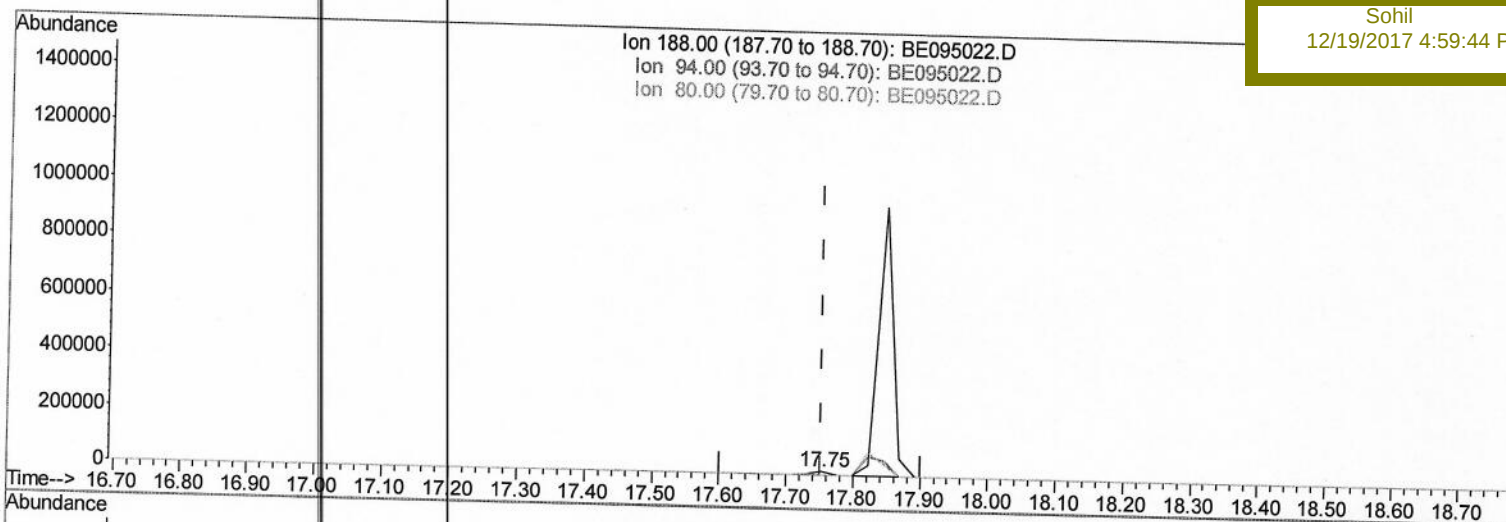

(10) Phenanthrene-d10 (I)

17.753min (+0.001) 0.40ng/ul m

response 23984

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	3.42#
80.00	11.80	2.82#
0.00	0.00	0.00

JU 12/19/17

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE121817\
 Data File : BE095022.D
 Acq On : 18 Dec 2017 22:26
 Operator : SJ/JU
 Sample : I6900-08
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Quant Time: Dec 19 06:06:14 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE121817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 19 04:08:16 2017
 Response via : Initial Calibration

Instrument :
 BNA_E
 ClientSampleId :
 F9C07

Manual Integrations
 APPROVED

Sohil
 12/19/2017 4:59:44 PM

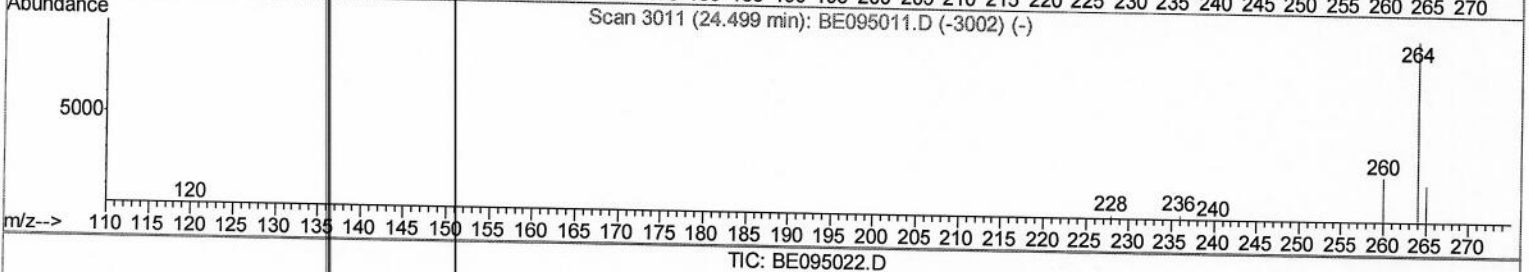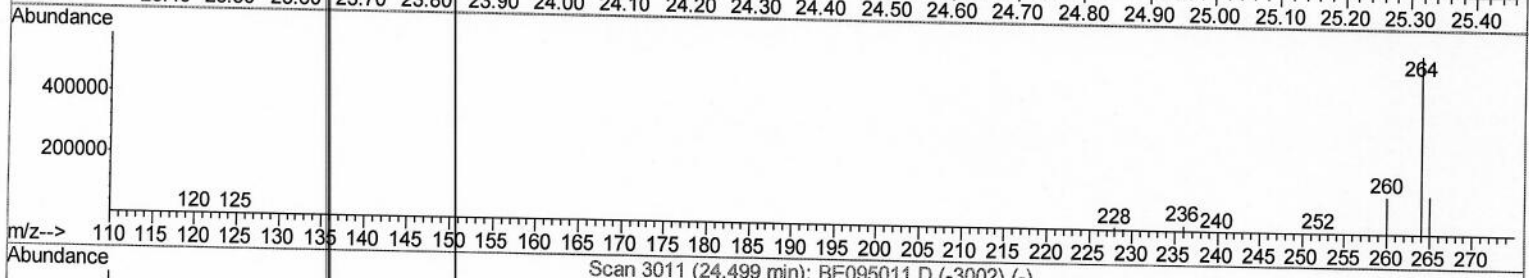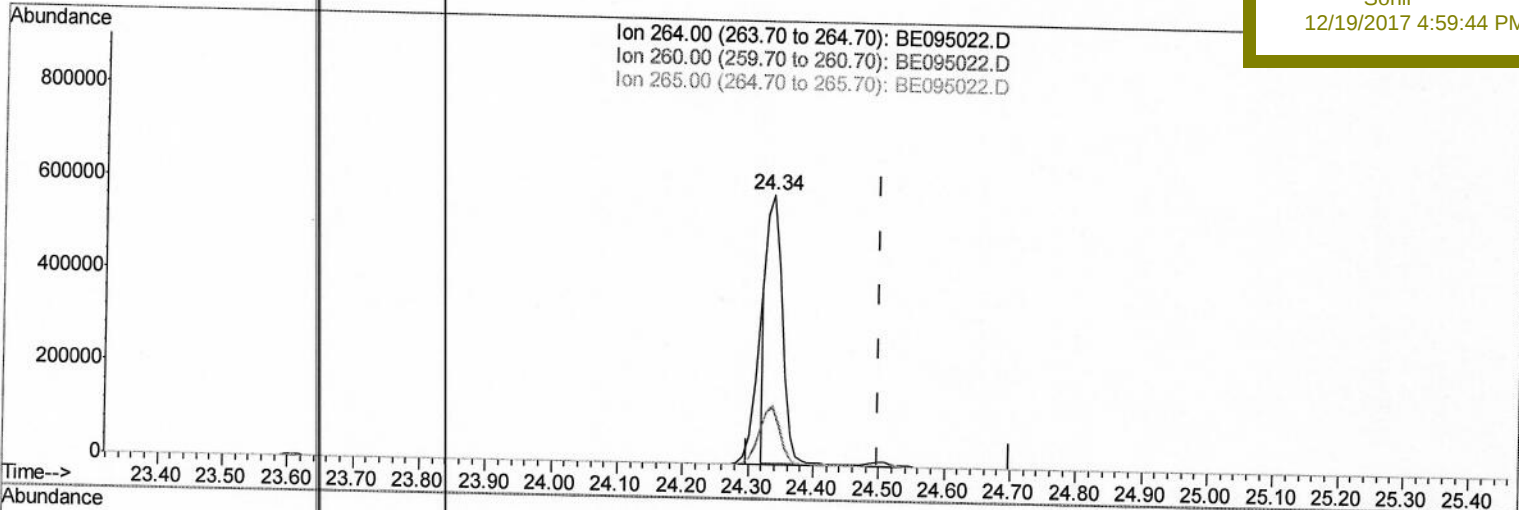

(20) Perylene-d12 (I)
 24.337min (-0.162) 0.40ng/ul
 response 987505

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	20.91#
265.00	103.50	21.61#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE121817\
 Data File : BE095022.D
 Acq On : 18 Dec 2017 22:26
 Operator : SJ/JU
 Sample : I6900-08
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :

BNA_E

ClientSampleId :

F9C07




Manual Integrations

APPROVED

Sohil

12/19/2017 4:59:44 PM

Quant Time: Dec 19 06:06:14 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE121817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 19 04:08:16 2017
 Response via : Initial Calibration

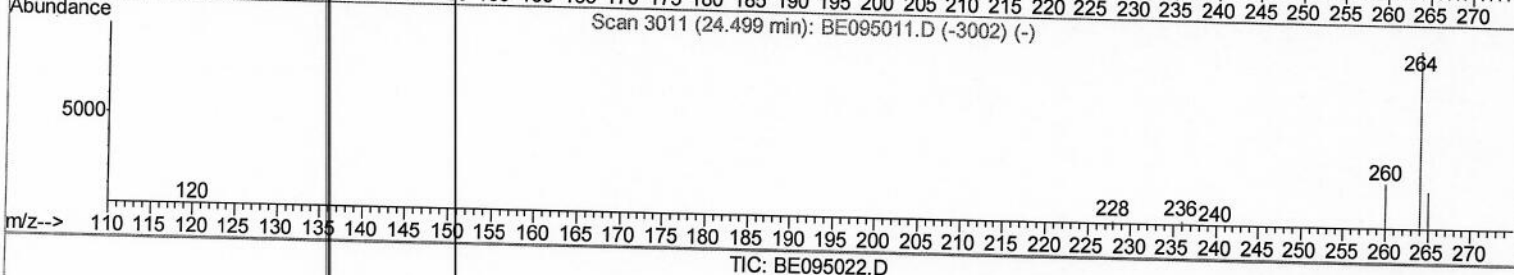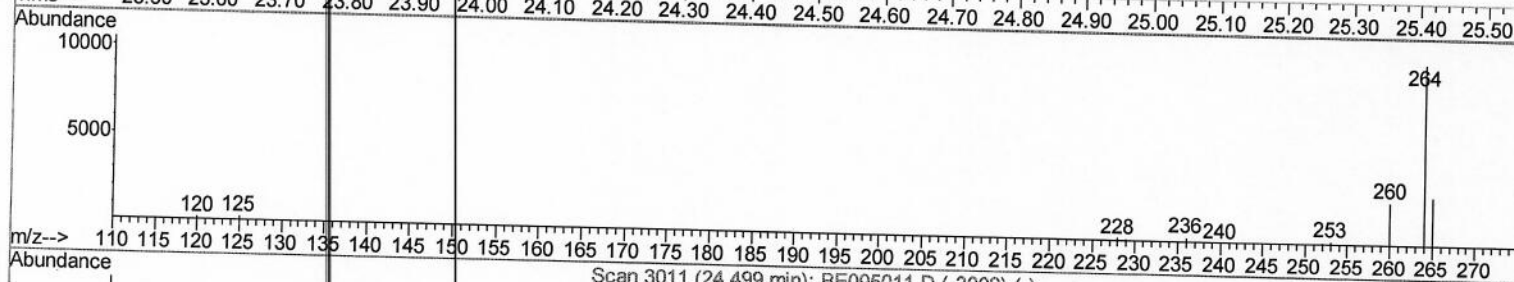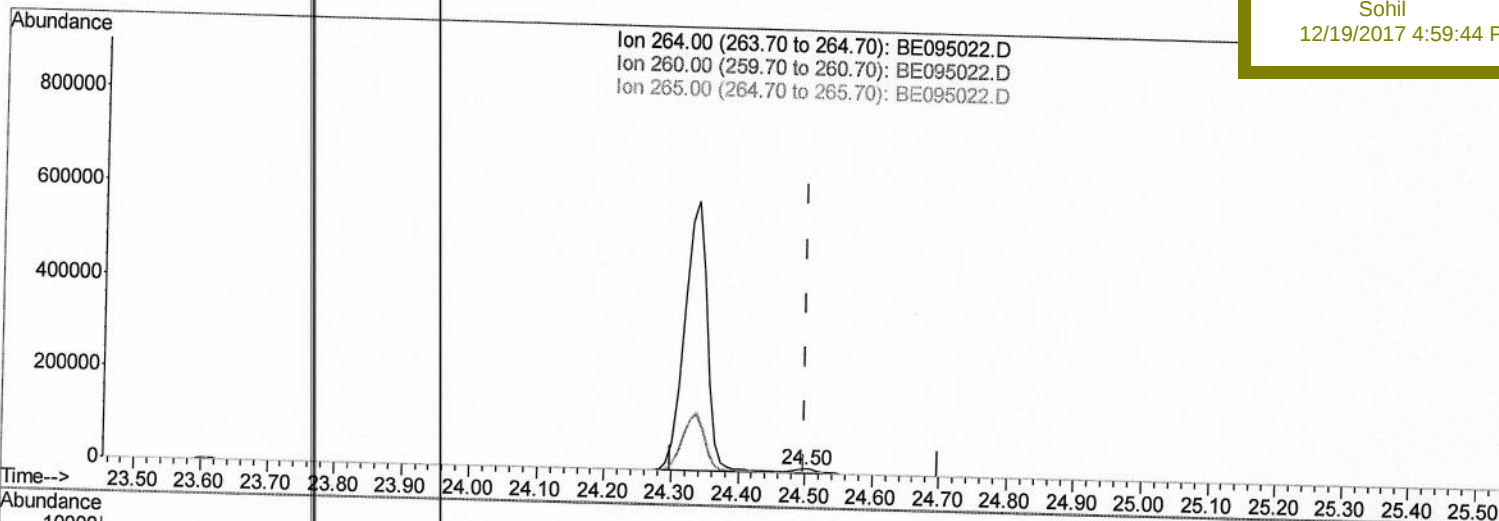

(20) Perylene-d12 (I)

24.499min (+0.000) 0.40ng/ul m

response 19020

Ion Exp% Act%

264.00 100 100

260.00 30.10 24.10

265.00 103.50 27.56#

0.00 0.00 0.00

JU 12/19/17

Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE121817\
 Data File : BE095022.D
 Acq On : 18 Dec 2017 22:26
 Operator : SJ/JU
 Sample : I6900-08
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Quant Time: Dec 19 06:07:02 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE121817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 19 04:08:16 2017
 Response via : Initial Calibration

Instrument :
 BNA_E
 Client Sample Id :
 F9C07

Manual Integrations
 APPROVED

Sohil
 12/19/2017 4:59:44 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.46	152	5194	0.40	ng/ul	0.00
2) Naphthalene-d8	11.29	136	17426	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.05	164	11022	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.75	188	23984m	0.40	ng/ul	0.00
16) Chrysene-d12	21.84	240	22857	0.40	ng/ul	0.00
20) Perylene-d12	24.50	264	19020m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.85	152	7506	0.26	ng/ul	0.00
14) Fluoranthene-d10	19.73	212	20354	0.27	ng/ul	0.00

Target Compounds

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SJU
 12/19/17

Data Path : Z:\HPCHEM1\BNA E\DATA\BE121817\
Data File : BE095022.D
Acq On : 18 Dec 2017 22:26
Operator : SJ/JU
Sample : I6900-08
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Dec 19 06:07:02 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE121817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 19 04:08:16 2017
Response via : Initial Calibration

Instrument :
BNA_E
ClientSampleId :
F9C07

Manual Integrations
APPROVED

Sohil
12/19/2017 4:59:44 PM

