
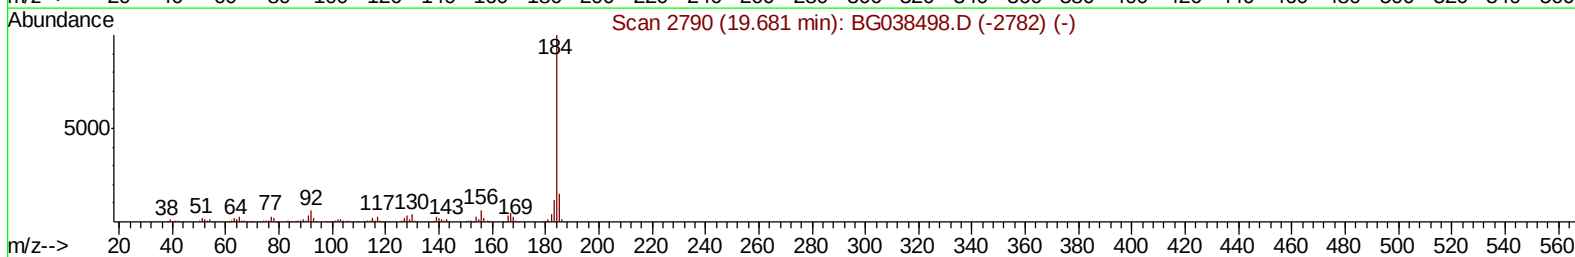
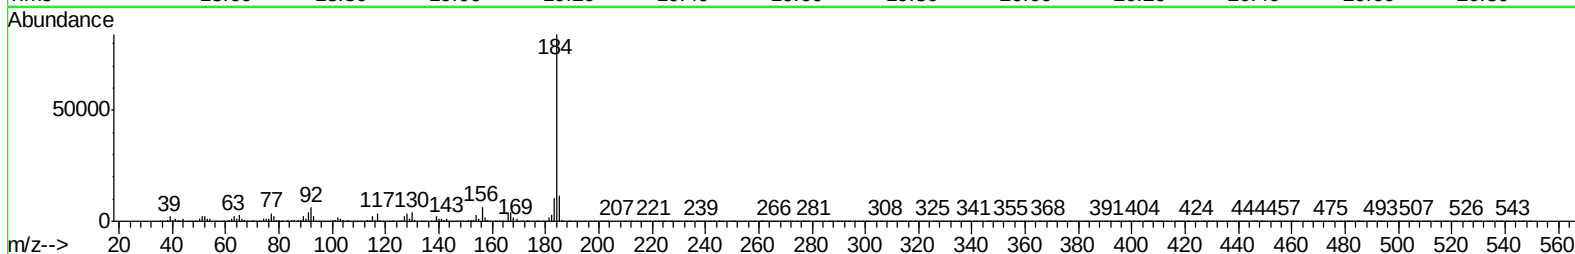


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE121818\
 Data File : BE098508.D
 Acq On : 18 Dec 2018 8:38
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 19 08:16:16 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 12 15:26:27 2018
 Response via : Initial Calibration

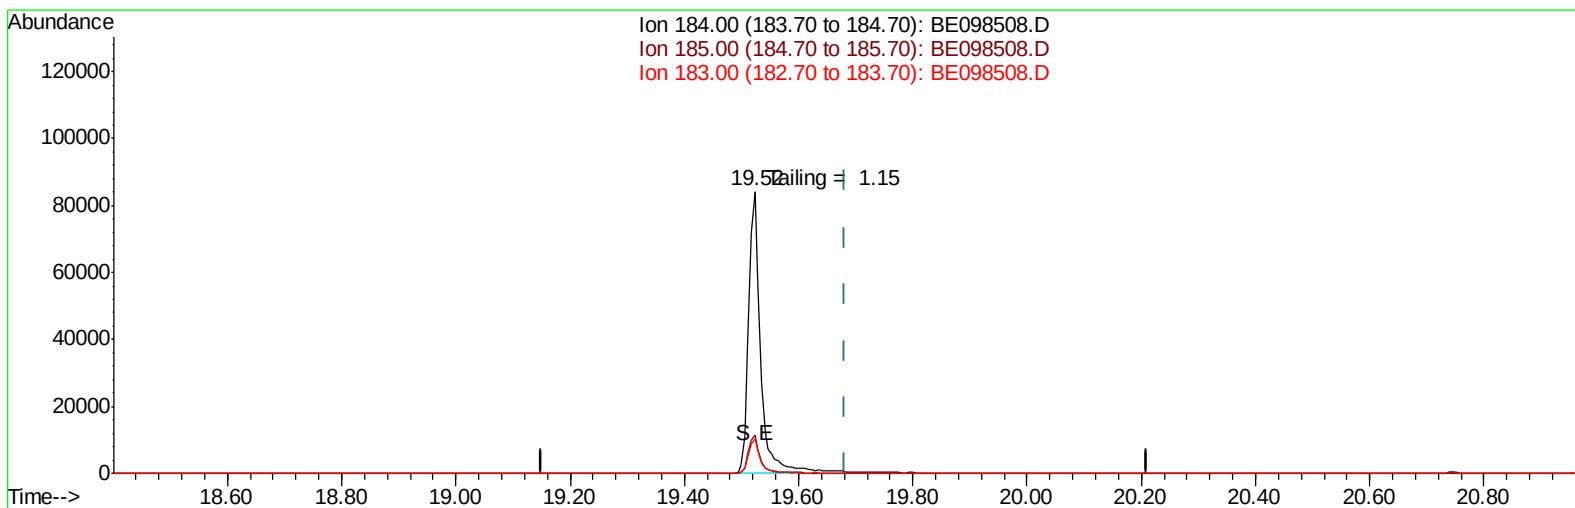

TIC: BE098508.D

(77) Benzidine




19.523min (-0.158) 413588.66ng

response 122315

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	13.51
183.00	12.00	12.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE121818\
Data File : BE098508.D
Acq On : 18 Dec 2018 8:38
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 19 08:16:16 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 15:26:27 2018
Response via : Initial Calibration

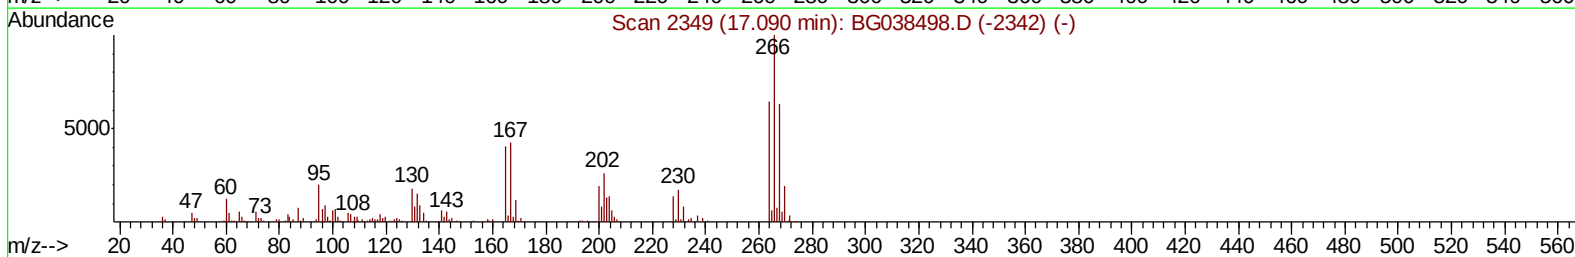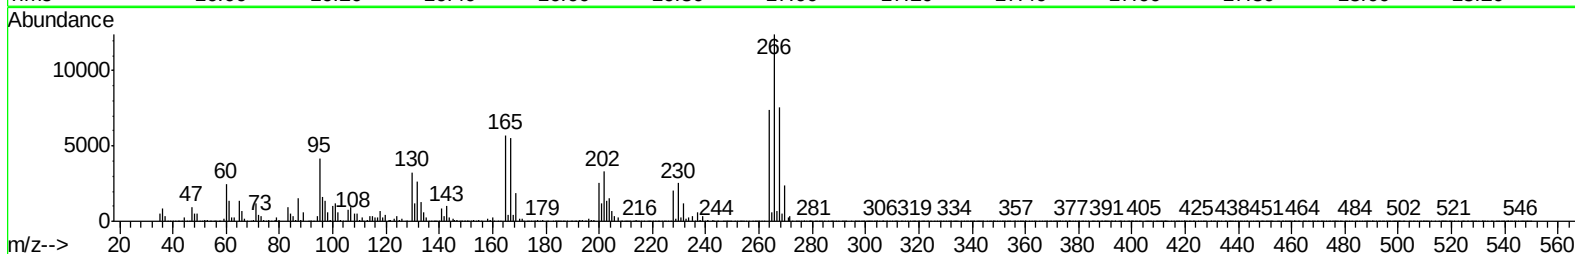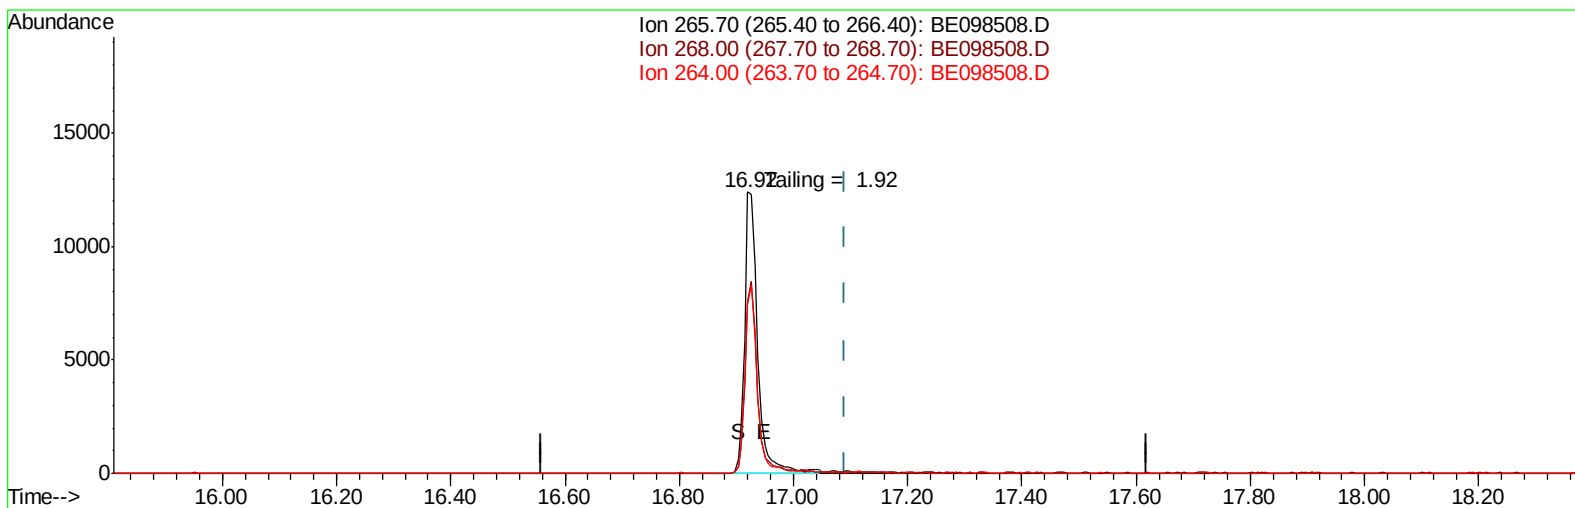

TIC: BE098508.D

(70) Pentachlorophenol (C)

16.920min (-0.170) 259353.55ng

response 19421

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	61.15
264.00	70.90	59.93
0.00	0.00	0.00