

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE121818\
 Data File : BE098519.D
 Acq On : 18 Dec 2018 19:04
 Operator : SJ/JU
 Sample : J6358-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 BP-FW-MW02-20181211

Quant Time: Dec 19 03:24:46 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE121018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 10 14:59:55 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	955	0.40	ng	-0.01
7) Naphthalene-d8	10.65	136	4609	0.40	ng	-0.01
13) Acenaphthene-d10	14.51	164	3305	0.40	ng	-0.01
19) Phenanthrene-d10	17.27	188	7941	0.40	ng	-0.01
27) Chrysene-d12	21.45	240	8940	0.40	ng	-0.01
34) Perylene-d12	23.99	264	8493	0.40	ng	-0.03
System Monitoring Compounds						
4) 2-Fluorophenol	5.45	112	520	0.23	ng	0.00
5) Phenol-d6	7.04	99	467	0.15	ng	-0.01
8) Nitrobenzene-d5	9.03	82	1415	0.34	ng	0.01
11) 2-Methylnaphthalene-d10	12.25	152	3126	0.42	ng	-0.01
14) 2,4,6-Tribromophenol	16.01	330	702	0.58	ng	-0.01
15) 2-Fluorobiphenyl	13.13	172	7210	0.52	ng	-0.01
25) Fluoranthene-d10	19.30	212	41243	0.40	ng	-0.01
29) Terphenyl-d14	19.89	244	10790	0.50	ng	-0.02
Target Compounds						Qvalue
32) Bis(2-ethylhexyl)phthalate	21.35	149	5364	0.104	ng	# 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE121818\
Data File : BE098519.D
Acq On : 18 Dec 2018 19:04
Operator : SJ/JU
Sample : J6358-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-FW-MW02-20181211

Quant Time: Dec 19 03:24:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE121018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 10 14:59:55 2018
Response via : Initial Calibration

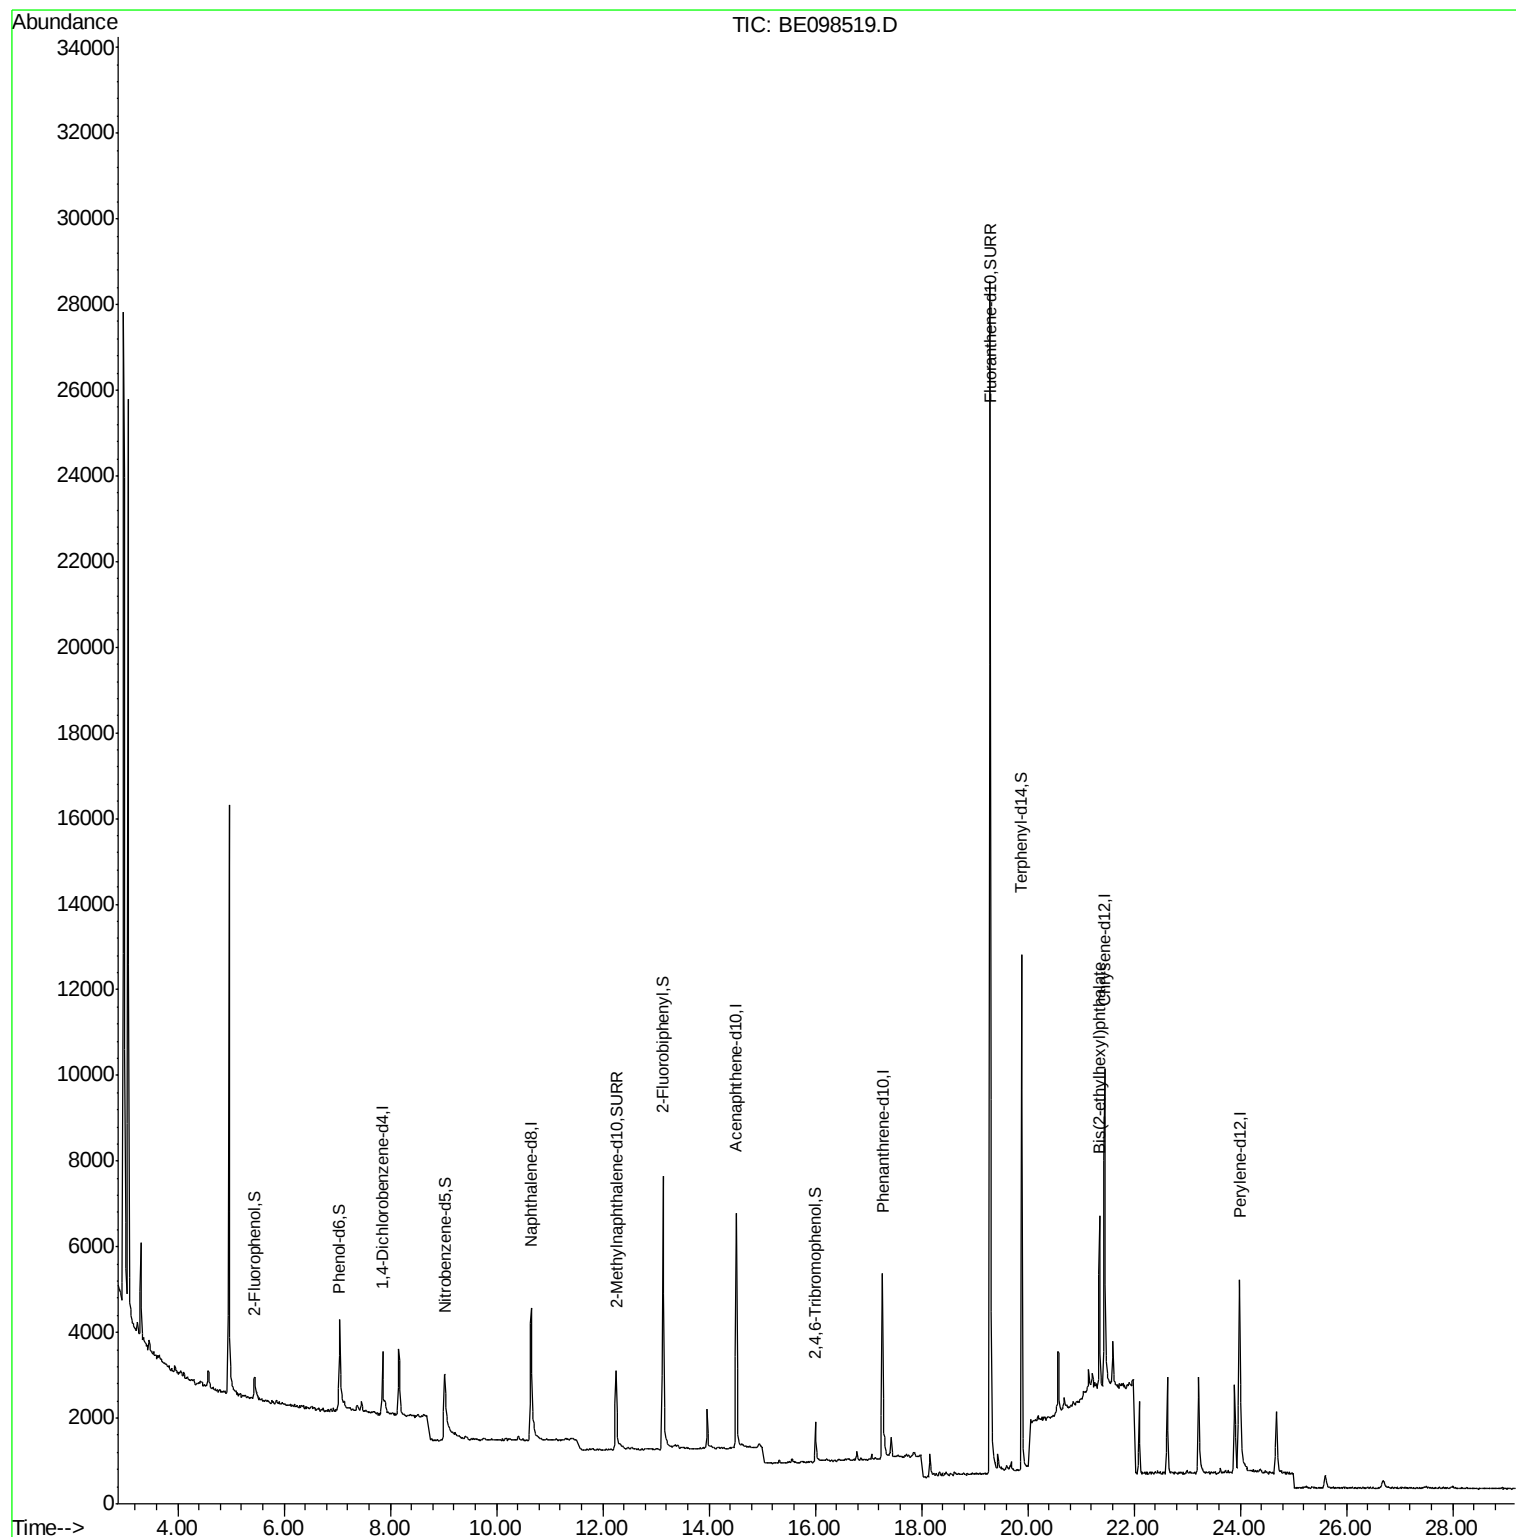



#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 7.85 min Scan# 433

Delta R.T. -0.01 min

Lab File: BE098519.D

Acq: 18 Dec 2018 19:04

Instrument :

BNA_E

ClientSampleId :

BP-FW-MW02-20181211


Tot Ion:152 Resp: 955

Ion Ratio Lower Upper

152 100

150 144.5 124.2 186.4


115 66.8 53.9 80.9

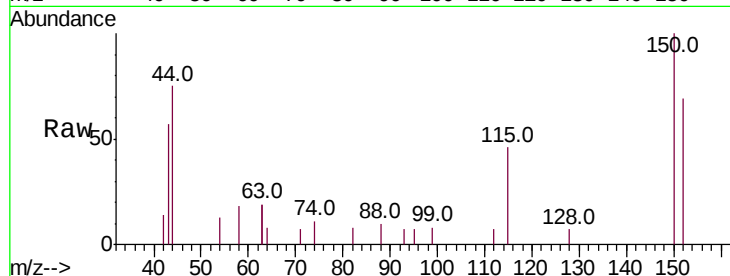



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

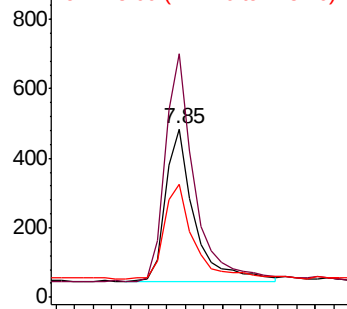

Time-->

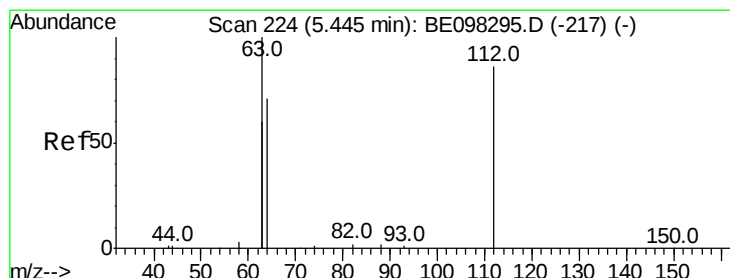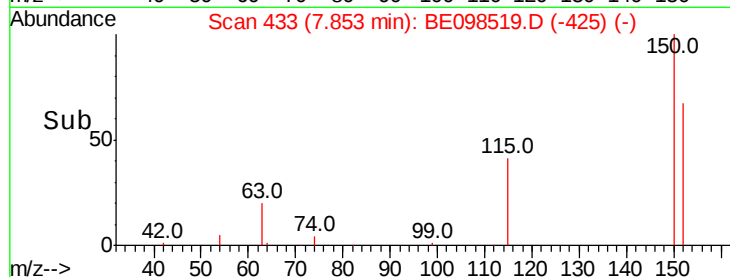

#4

2-Fluorophenol

Concen: 0.233 ng

RT: 5.45 min Scan# 224

Delta R.T. 0.00 min

Lab File: BE098519.D

Acq: 18 Dec 2018 19:04


Tgt Ion:112 Resp: 520

Ion Ratio Lower Upper

112 100

64 69.8 59.8 89.8


63 141.3 133.7 200.5

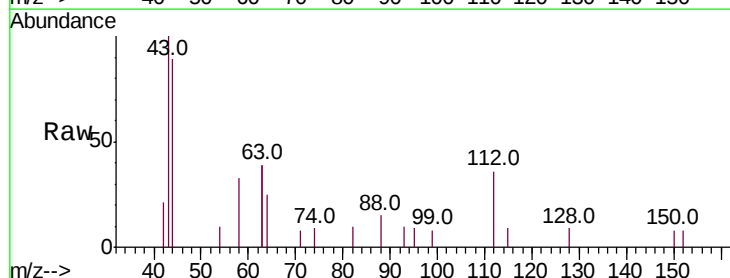


Abundance Ion 112.00 (111.70 to 112.70): E


Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

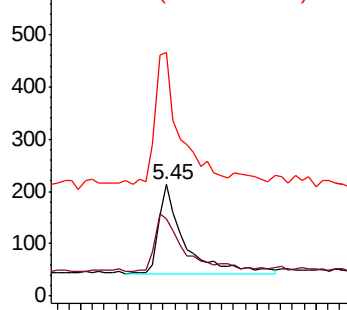

Time-->

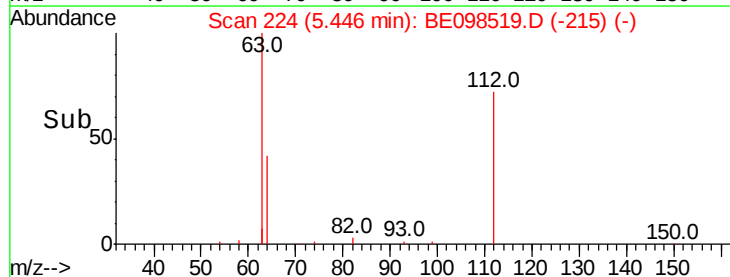

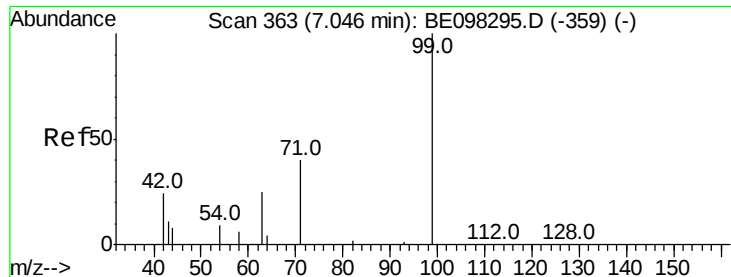

#5

Phenol-d6

Concen: 0.148 ng

RT: 7.04 min Scan# 362

Delta R.T. -0.01 min

Lab File: BE098519.D

Acq: 18 Dec 2018 19:04

Instrument :

BNA_E

ClientSampleId :

BP-FW-MW02-20181211





Tot Ion: 99 Resp: 467

Ion Ratio Lower Upper

99 100

42 0.0 26.3 39.5#

71 40.5 33.6 50.4

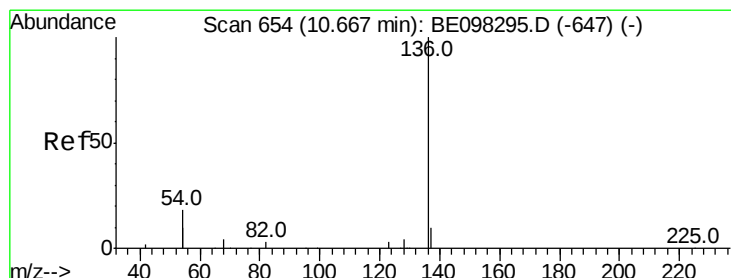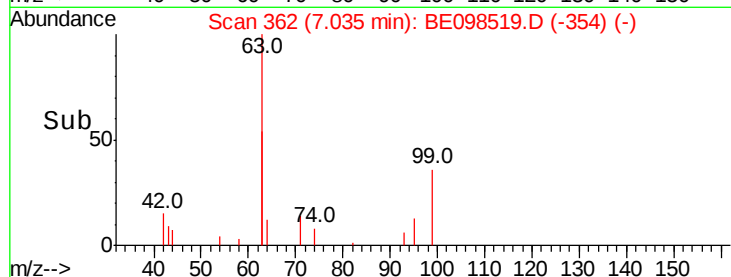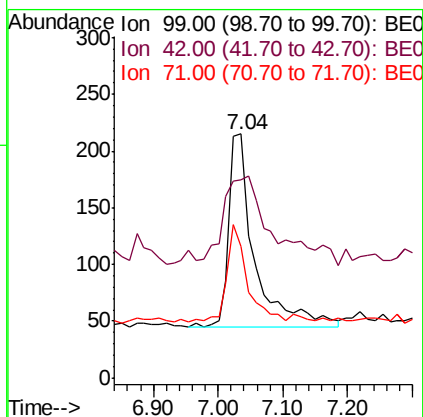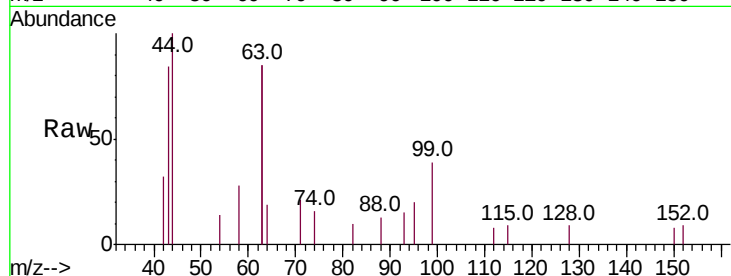

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.65 min Scan# 653

Delta R.T. -0.01 min

Lab File: BE098519.D

Acq: 18 Dec 2018 19:04

Tgt Ion: 136 Resp: 4609




Ion Ratio Lower Upper

136 100

137 12.8 9.2 13.8

54 40.7 28.4 42.6

68 7.2 5.4 8.0

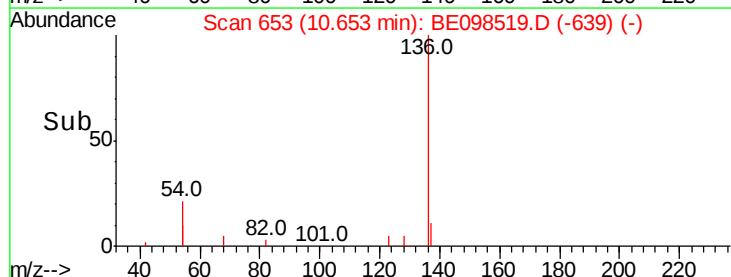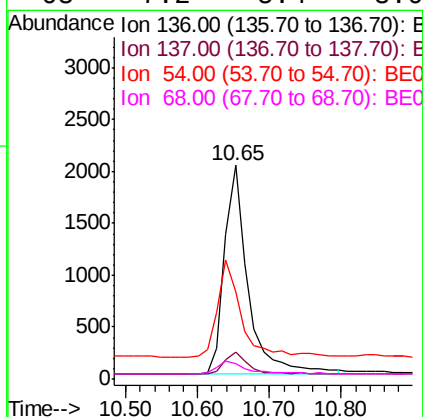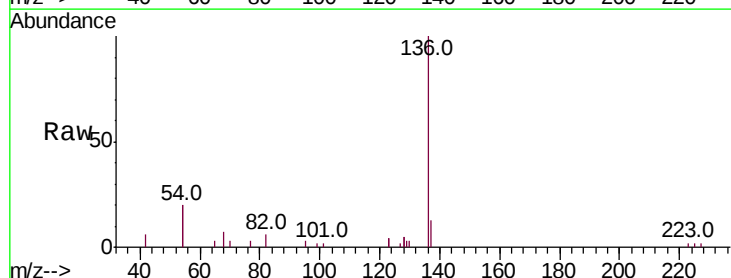



#8

Nitrobenzene-d5

Concen: 0.337 ng

RT: 9.03 min Scan# 528

Delta R.T. 0.01 min

Lab File: BE098519.D

Acq: 18 Dec 2018 19:04

Instrument :

BNA_E

ClientSampleId :

BP-FW-MW02-20181211


Tot Ion: 82 Resp: 1415

Ion Ratio Lower Upper

82 100

128 168.7 102.4 153.6#



54 264.8 221.8 332.8

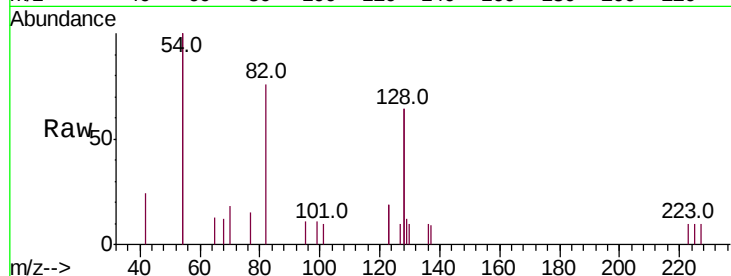

Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0

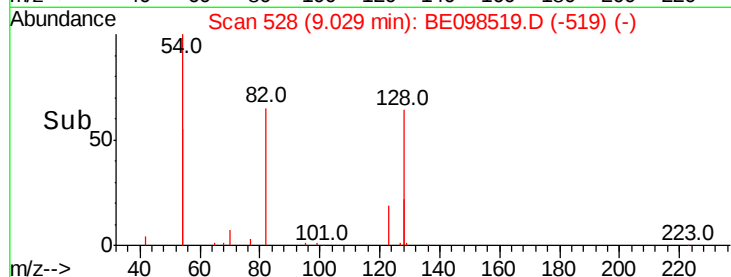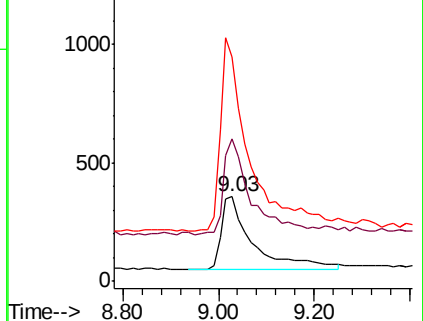

#11

2-Methylnaphthalene-d10

Concen: 0.417 ng

RT: 12.25 min Scan# 766

Delta R.T. -0.01 min

Lab File: BE098519.D


Acq: 18 Dec 2018 19:04

Tgt Ion:152 Resp: 3126

Ion Ratio Lower Upper



152 100


151 18.9 16.2 24.4

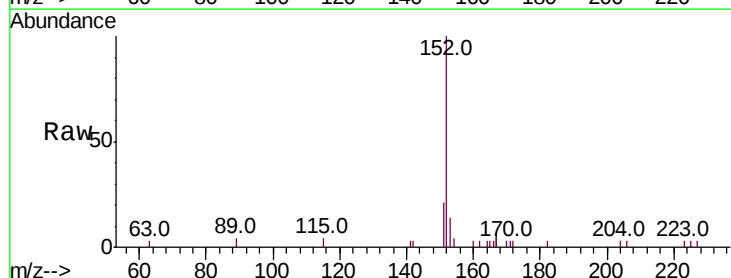

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

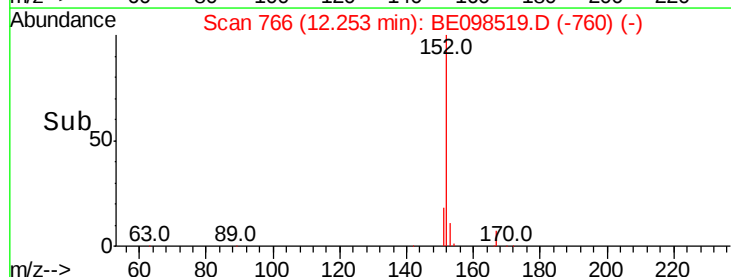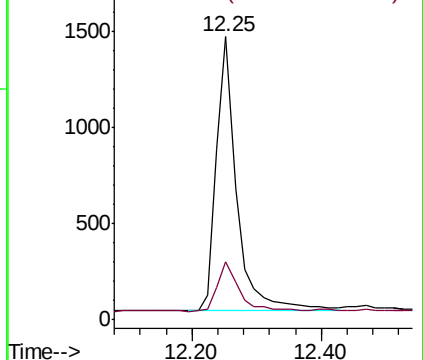

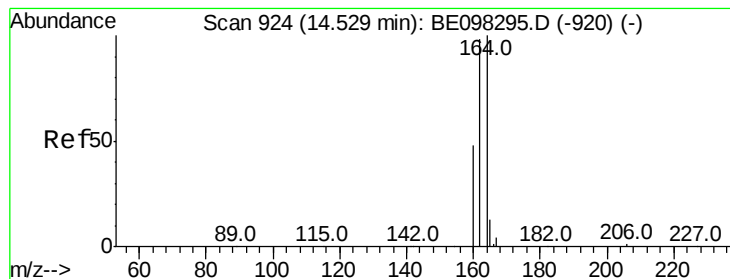

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.51 min Scan# 923

Delta R.T. -0.01 min

Lab File: BE098519.D

Acq: 18 Dec 2018 19:04

Instrument :

BNA_E

ClientSampleId :

BP-FW-MW02-20181211


Tot Ion:164 Resp: 3305

Ion Ratio Lower Upper

164 100

162 95.7 77.6 116.4




160 46.6 36.0 54.0

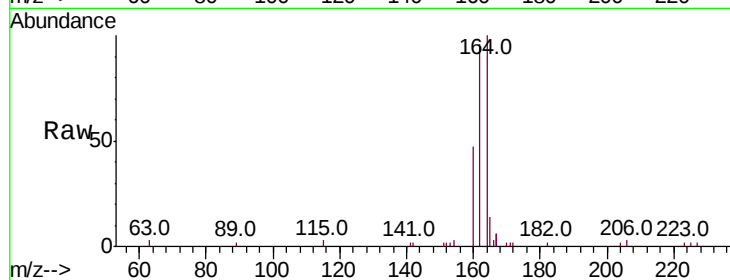

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

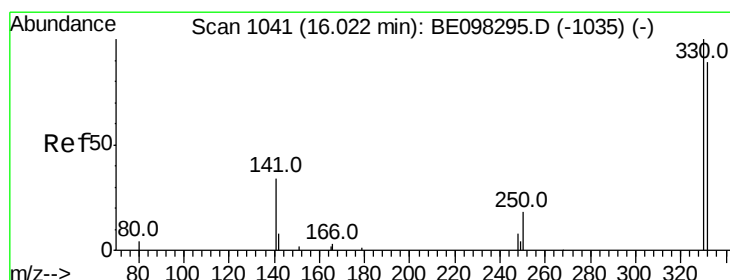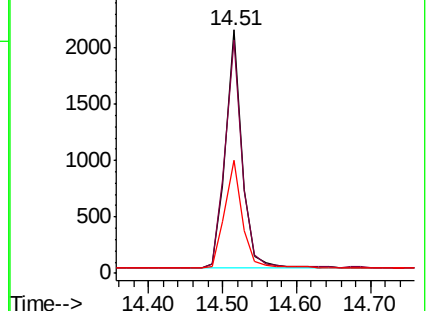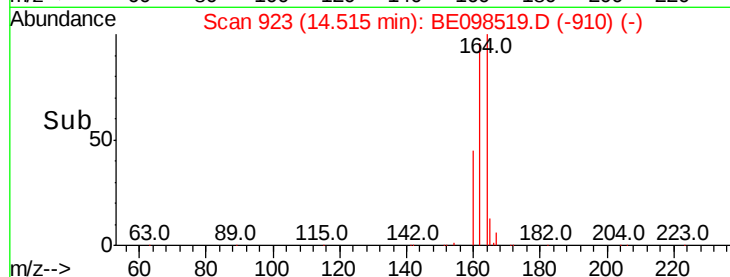

#14

2,4,6-Tribromophenol

Concen: 0.579 ng

RT: 16.01 min Scan# 1040

Delta R.T. -0.01 min

Lab File: BE098519.D

Acq: 18 Dec 2018 19:04


Tgt Ion:330 Resp: 702

Ion Ratio Lower Upper

330 100

332 92.3 76.2 114.4



141 41.3 39.0 58.4

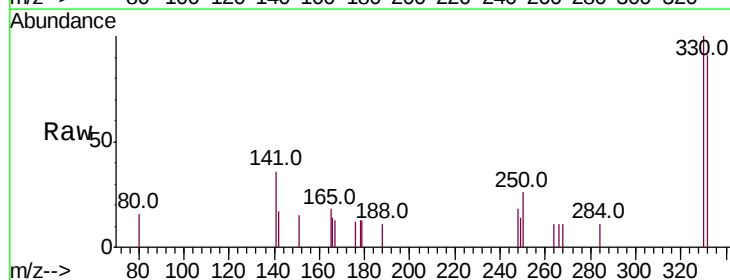


Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

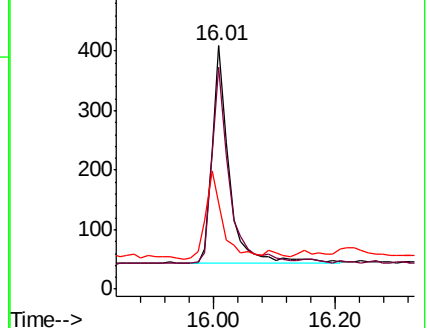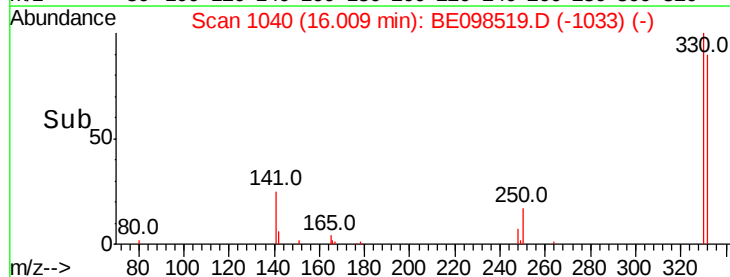


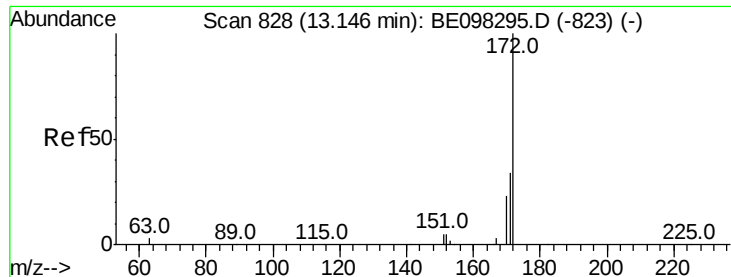




#15
2-Fluorobiphenyl
Concen: 0.517 ng
RT: 13.13 min Scan# 827
Delta R.T. -0.01 min
Lab File: BE098519.D
Acq: 18 Dec 2018 19:04

Instrument :
BNA_E
ClientSampleId :
BP-FW-MW02-20181211

Tot Ion:172 Resp: 7210
Ion Ratio Lower Upper
172 100
171 34.4 27.5 41.3
170 23.4 19.6 29.4

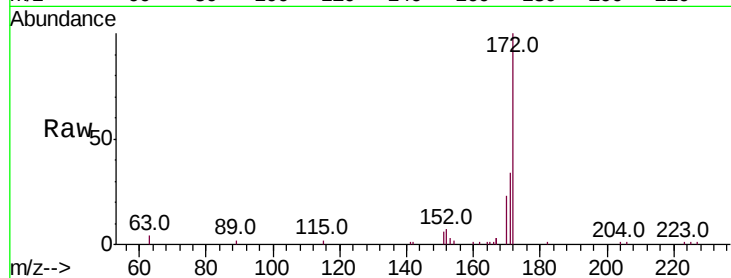


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

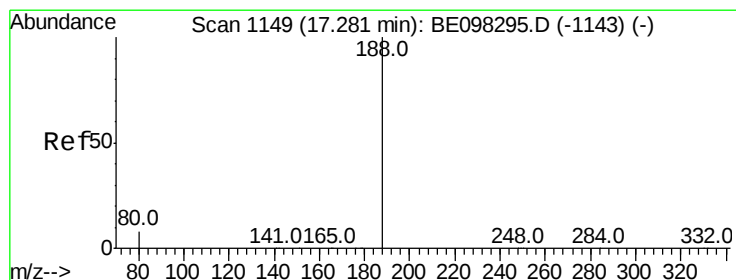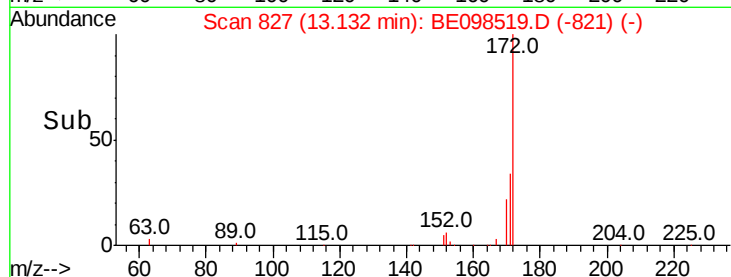
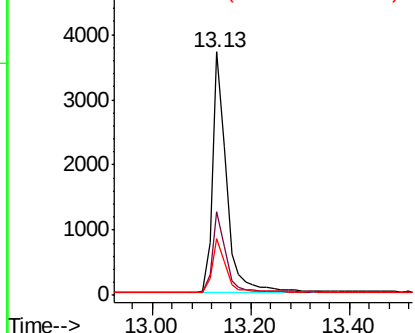



#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.27 min Scan# 1148
Delta R.T. -0.01 min
Lab File: BE098519.D
Acq: 18 Dec 2018 19:04

Tgt Ion:188 Resp: 7941
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 7.3 7.2 10.8

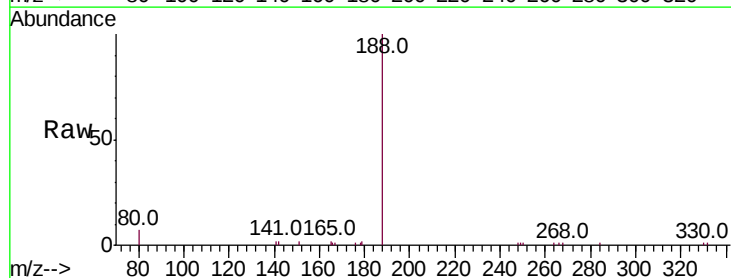

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BE0
Ion 80.00 (79.70 to 80.70): BE0

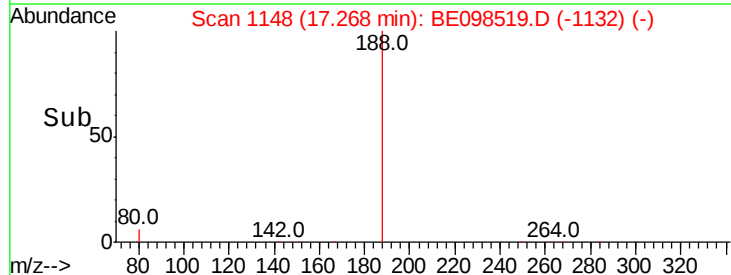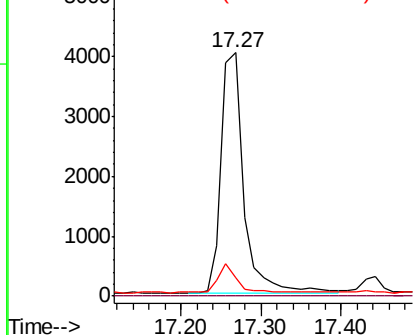

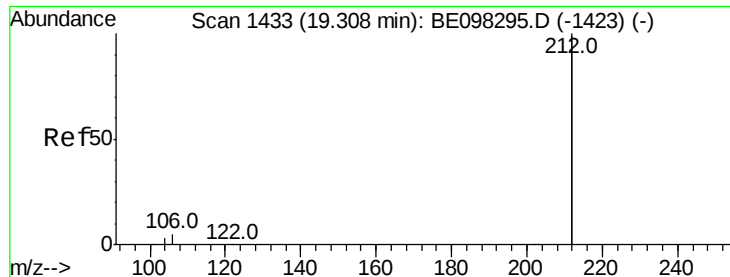

#25

Fluoranthene-d10

Concen: 0.405 ng

RT: 19.30 min Scan# 1431

Delta R.T. -0.01 min

Lab File: BE098519.D

Acq: 18 Dec 2018 19:04

Instrument :

BNA_E

ClientSampleId :

BP-FW-MW02-20181211


Tot Ion:212 Resp: 41243

Ion Ratio Lower Upper

212 100

106 2.4 2.2 3.2




104 1.4 1.3 1.9

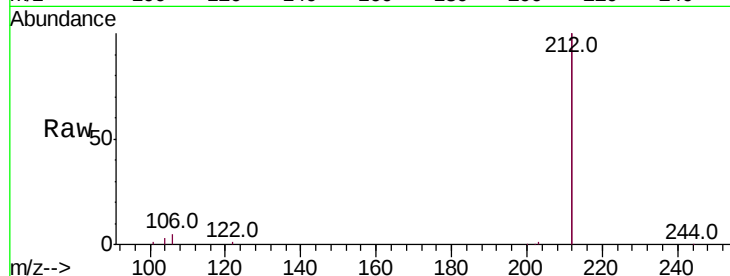

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

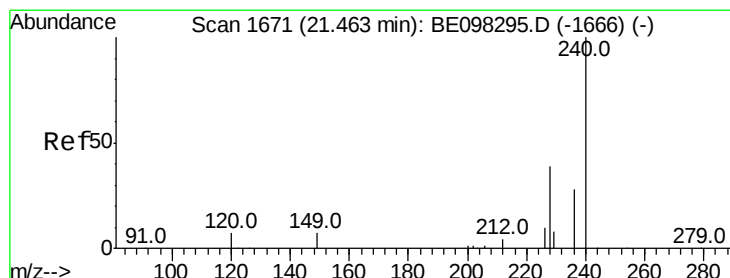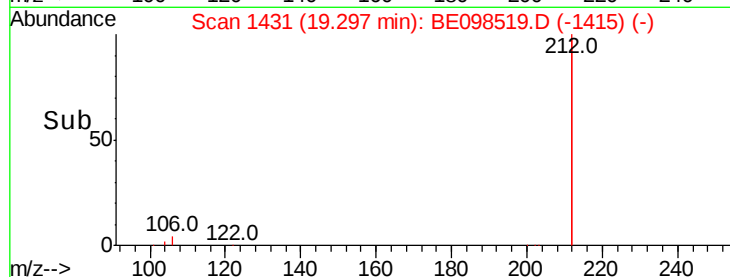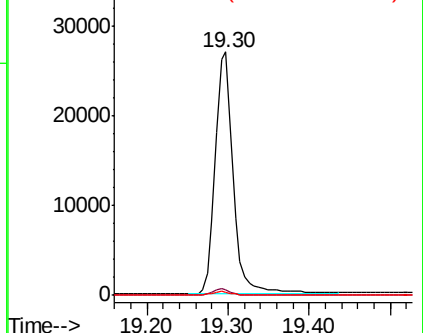

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.45 min Scan# 1670

Delta R.T. -0.01 min

Lab File: BE098519.D

Acq: 18 Dec 2018 19:04


Tgt Ion:240 Resp: 8940

Ion Ratio Lower Upper

240 100

120 6.5 9.5 14.3#



236 26.5 22.7 34.1

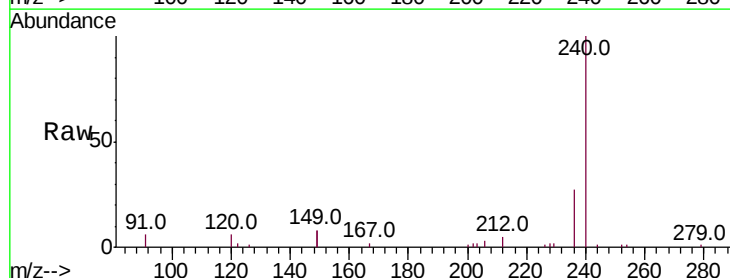


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

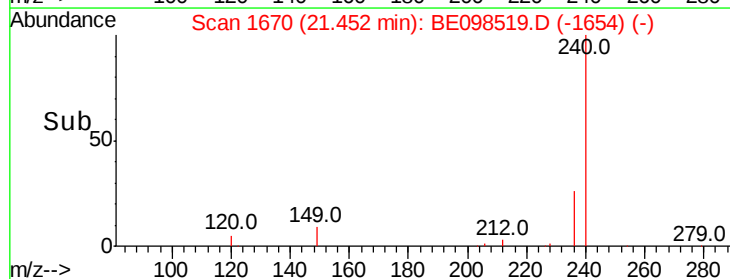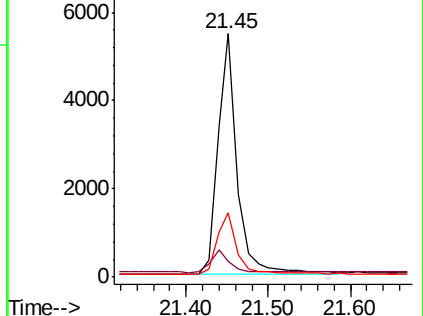

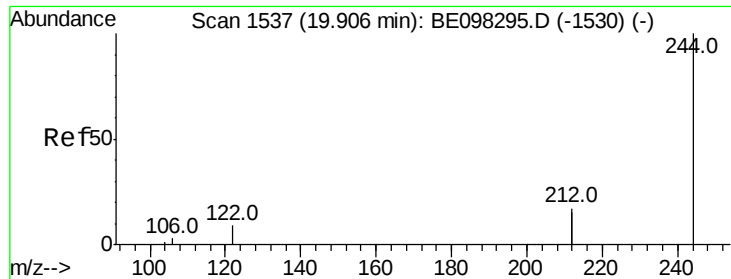

#29

Terphenyl-d14

Concen: 0.497 ng

RT: 19.89 min Scan# 1534

Delta R.T. -0.02 min

Lab File: BE098519.D

Acq: 18 Dec 2018 19:04

Instrument :

BNA_E

ClientSampleId :

BP-FW-MW02-20181211


Tot Ion:244 Resp: 10790

Ion Ratio Lower Upper

244 100

212 34.8 27.4 41.0




122 9.0 8.3 12.5

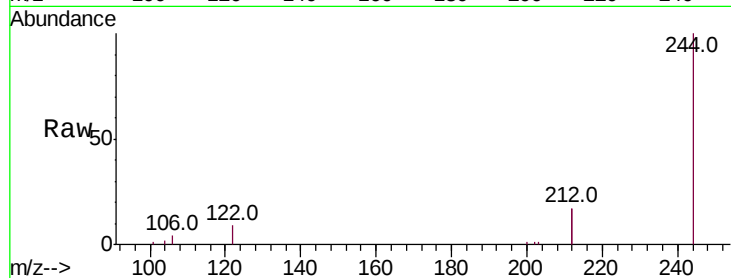

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

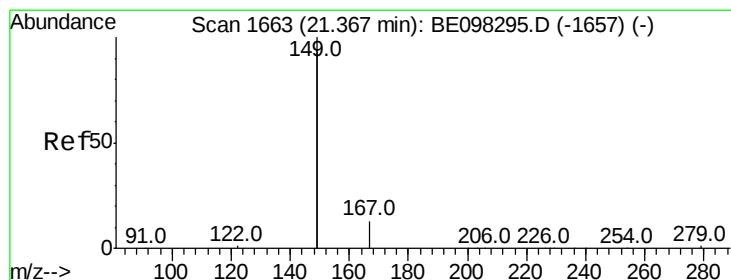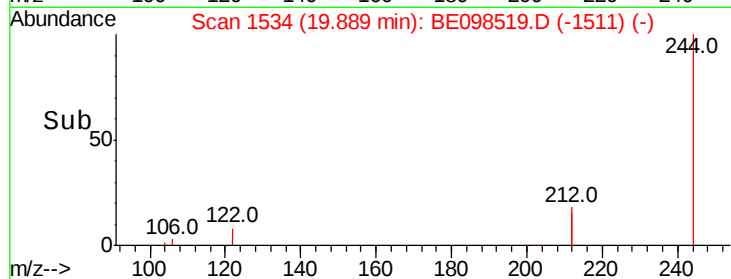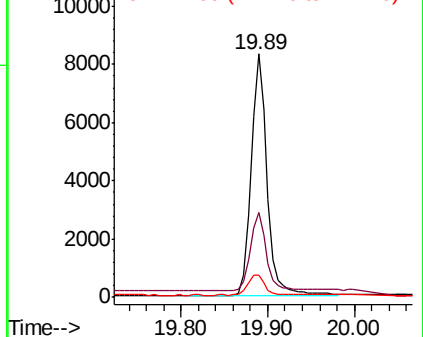

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.104 ng

RT: 21.35 min Scan# 1662

Delta R.T. -0.01 min

Lab File: BE098519.D

Acq: 18 Dec 2018 19:04


Tgt Ion:149 Resp: 5364

Ion Ratio Lower Upper

149 100

167 6.8 5.7 8.5



279 1.5 1.0 1.4#


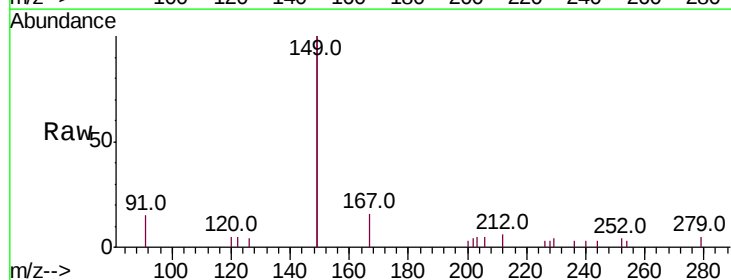


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

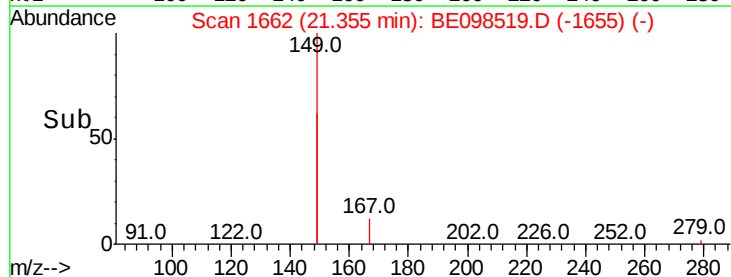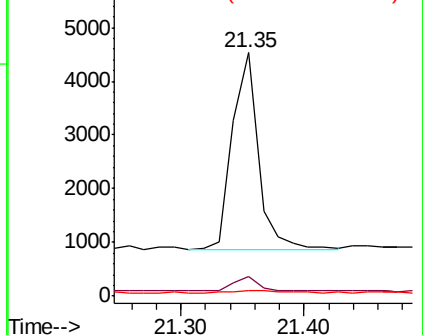

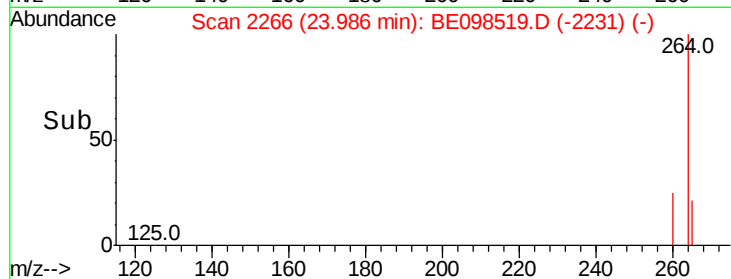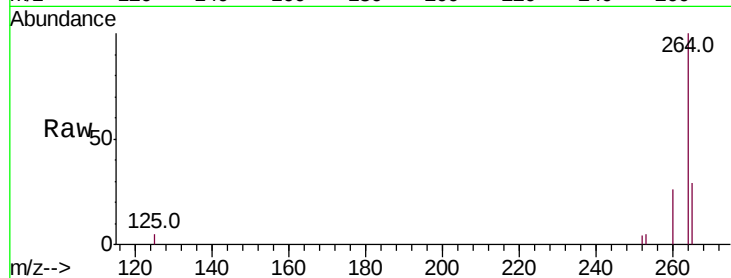

#34

Pervlene-d12

Concen: 0.400 ng

RT: 23.99 min Scan# 2266

Delta R.T. -0.03 min

Lab File: BE098519.D

Acq: 18 Dec 2018 19:04

Instrument :

BNA_E

ClientSampleId :

BP-FW-MW02-20181211

Tot Ion:264 Resp: 8493

Ion Ratio Lower Upper

264 100

260 25.9 20.2 30.2

265 29.1 25.2 37.8

