


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE121818\  
 Data File : BE098508.D  
 Acq On : 18 Dec 2018 8:38  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_E\METHODS\8270-SIM-BE121018.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Dec 10 14:59:55 2018

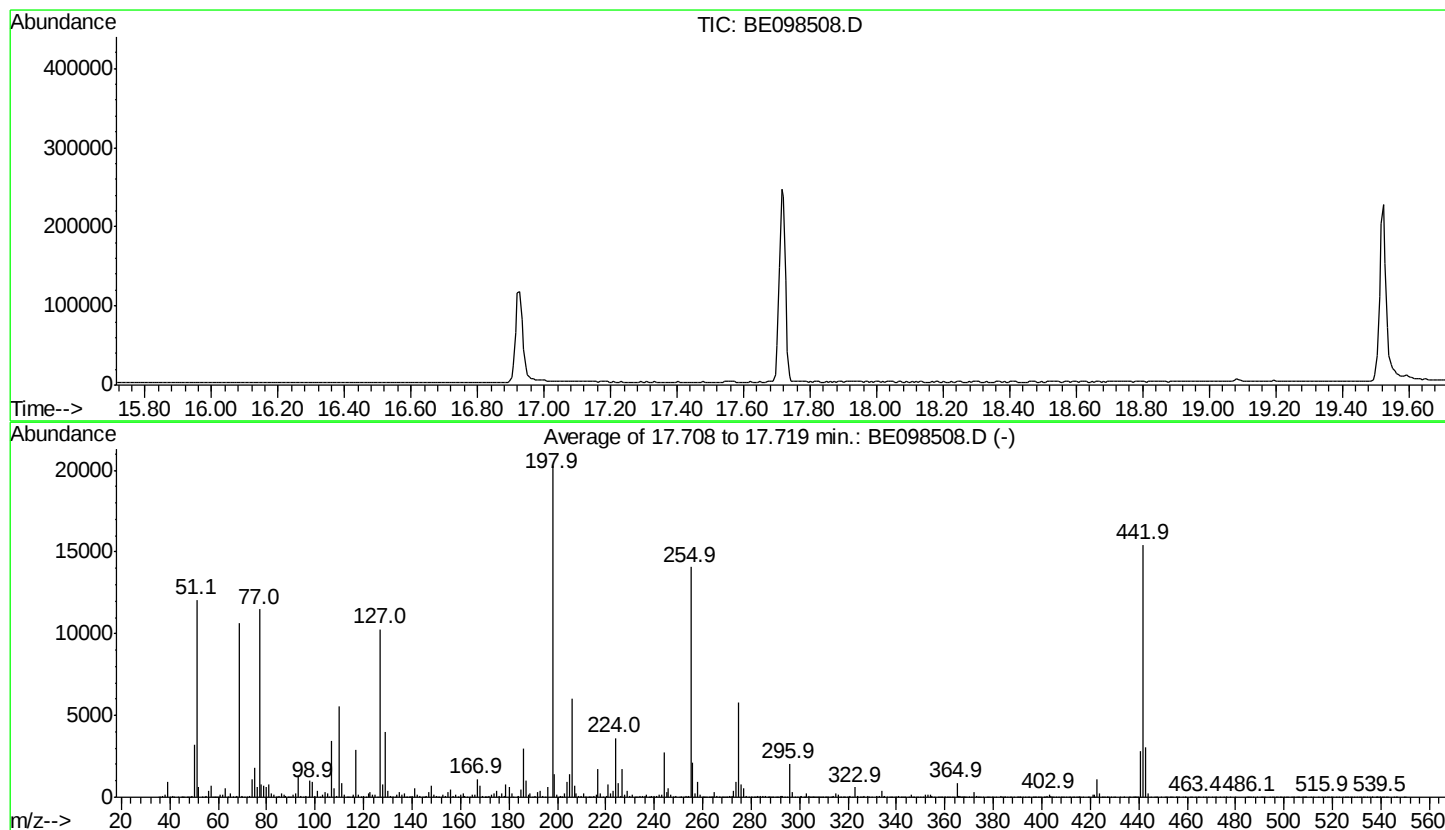

AutoFind: Scans 2573, 2574, 2575; Background Corrected with Scan 2566

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 59.5      | 12070   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.0       | 108     | PASS             |
| 69          | 198          | 0.00         | 100          | 52.4      | 10631   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.4       | 47      | PASS             |
| 127         | 198          | 10           | 80           | 50.7      | 10290   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 20278   | PASS             |
| 199         | 198          | 5            | 9            | 7.1       | 1443    | PASS             |
| 275         | 198          | 10           | 60           | 28.8      | 5831    | PASS             |
| 365         | 198          | 1            | 100          | 4.4       | 884     | PASS             |
| 441         | 198          | 0.01         | 100          | 13.8      | 2791    | PASS             |
| 442         | 198          | 50           | 100          | 76.1      | 15425   | PASS             |
| 443         | 442          | 15           | 24           | 19.7      | 3038    | PASS             |