
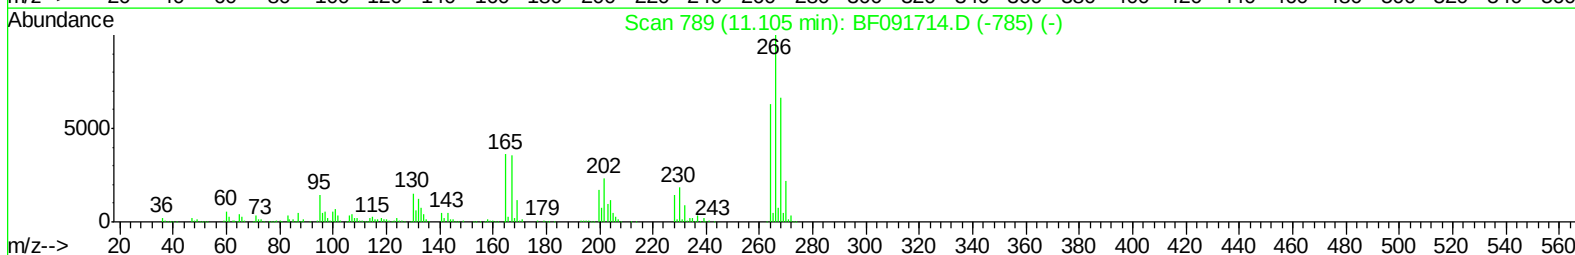
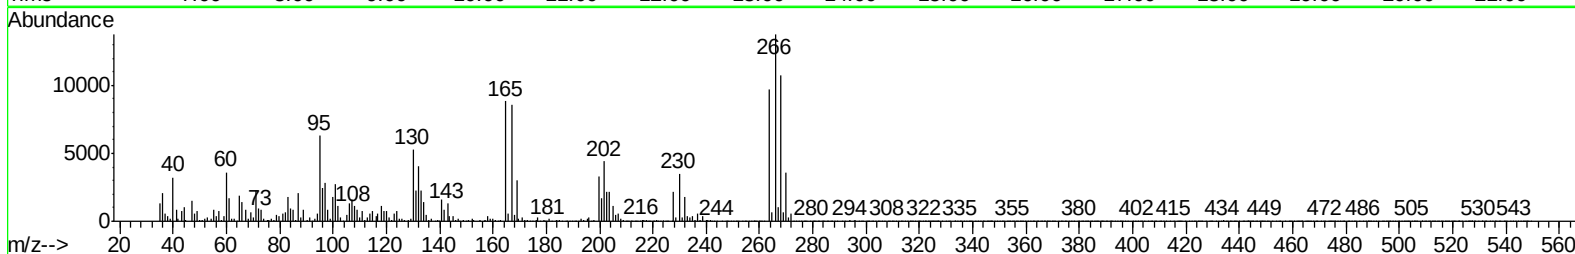


Data Path : Z:\HPCHEM1\BNA_E\Data\BE121916\
Data File : BE092599.D
Acq On : 19 Dec 2016 9:23
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 07:59:18 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 17 22:53:54 2016
Response via : Initial Calibration

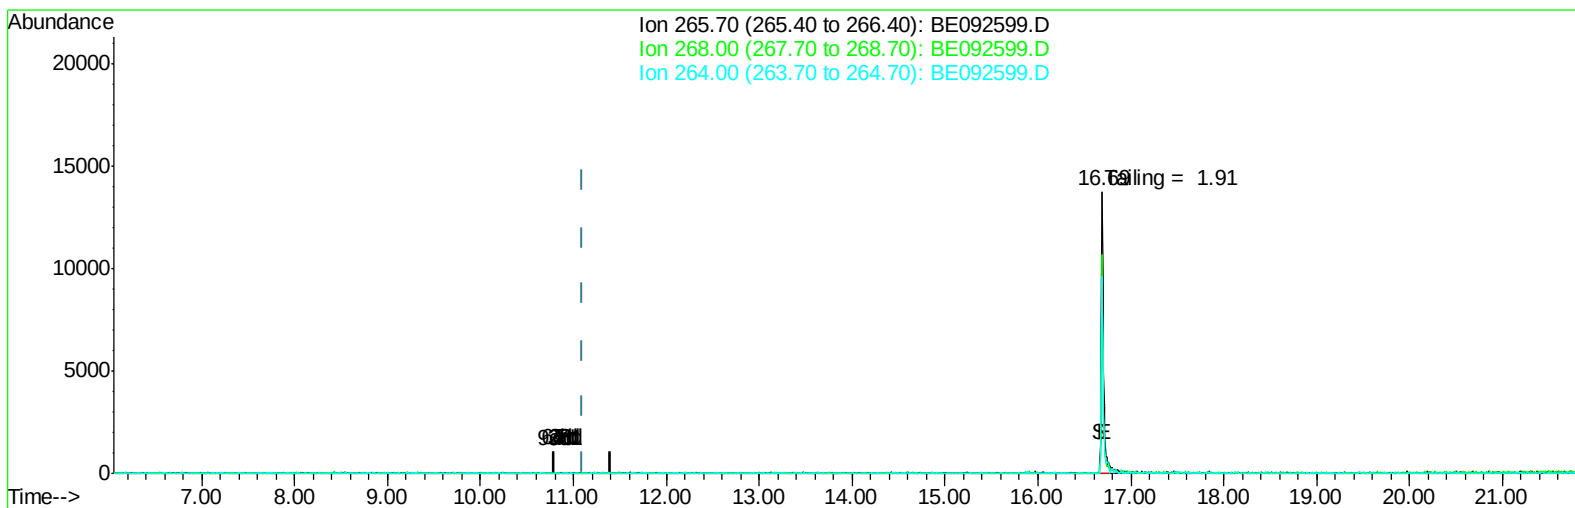

TIC: BE092599.D

(69) Pentachlorophenol (C)




16.689min (+5.584) 469678.08ng m

response 25064

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	77.87
264.00	62.90	70.23
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\Data\BE121916\
Data File : BE092599.D
Acq On : 19 Dec 2016 9:23
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 07:59:18 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 17 22:53:54 2016
Response via : Initial Calibration

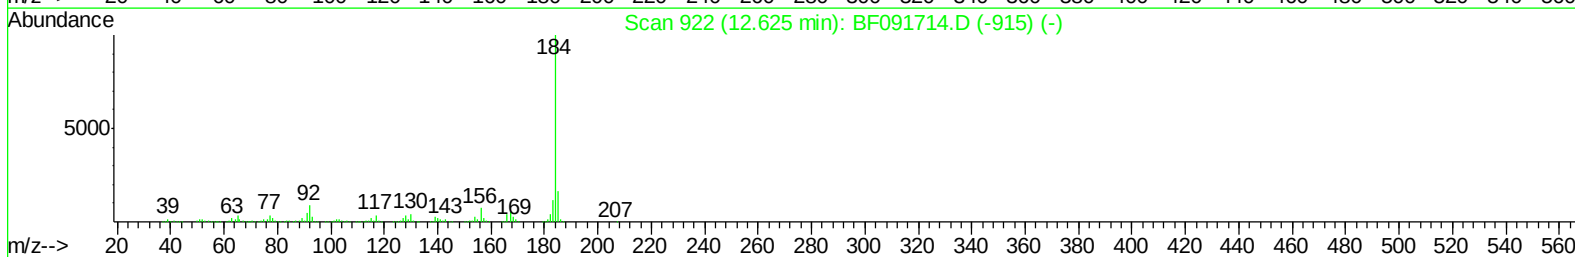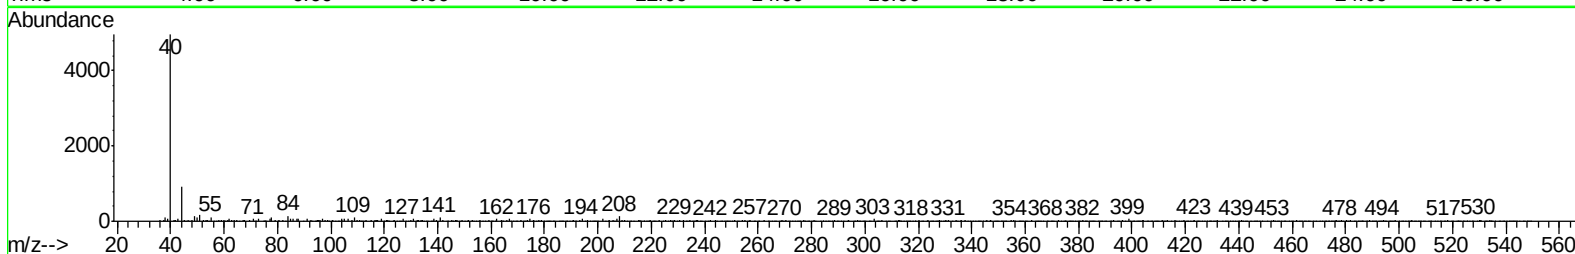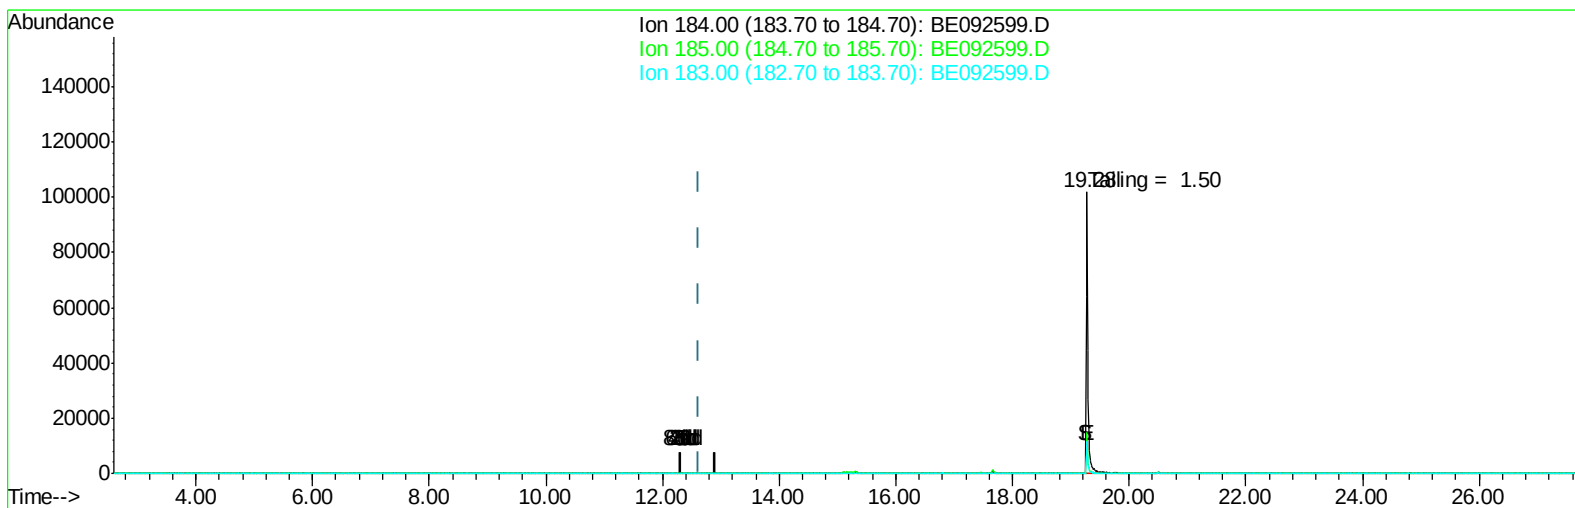

TIC: BE092599.D

(76) Benzidine

12.347min (-0.278) 24.81ng

response 10

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	100.00#
183.00	11.50	108.33#
0.00	0.00	0.00