


Data Path : Z:\HPCHEM1\BNA E\DATA\BE121916\
 Data File : BE092599.D
 Acq On : 19 Dec 2016 9:23
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE121916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 19 16:16:32 2016

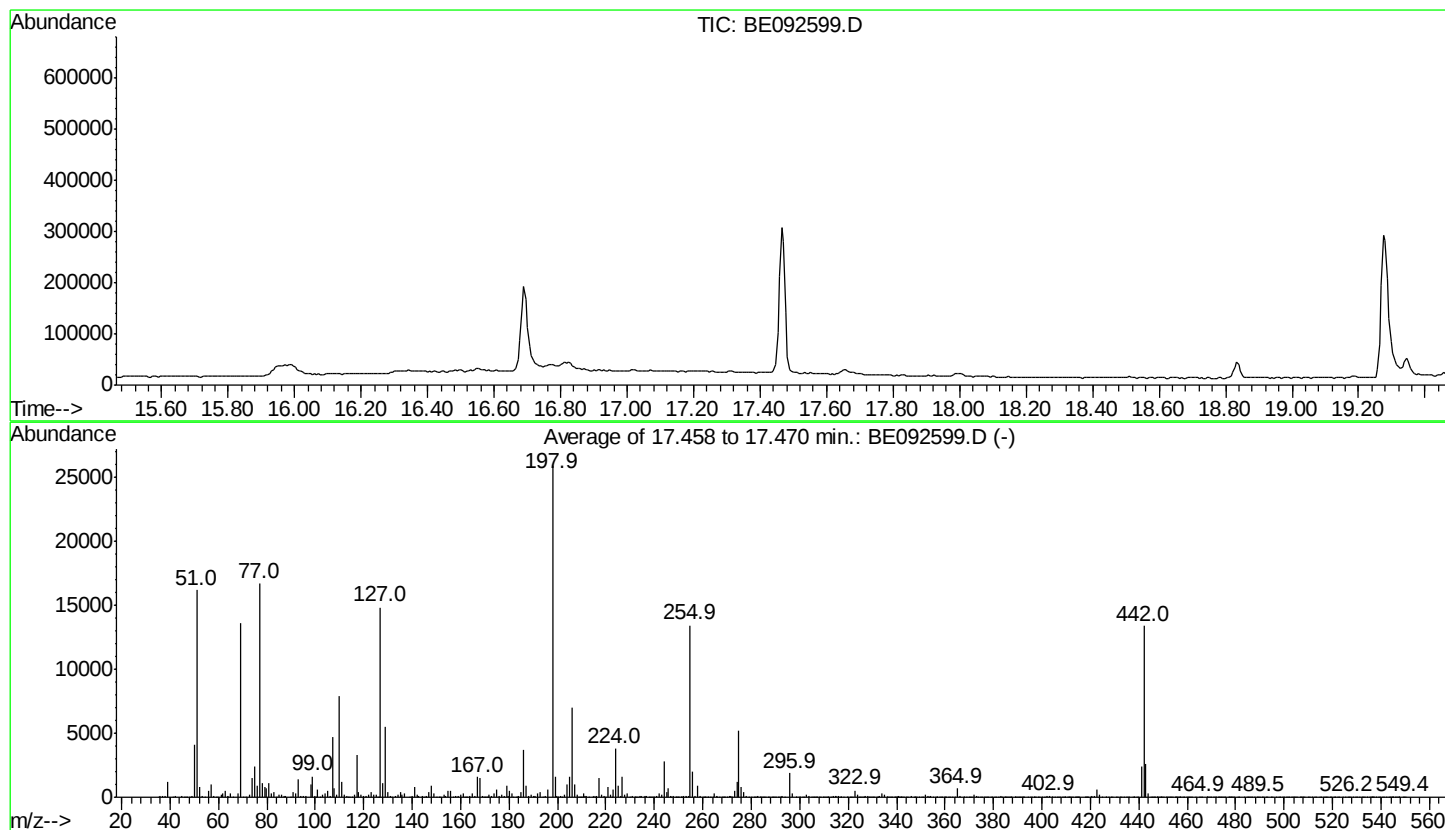

AutoFind: Scans 2531, 2532, 2533; Background Corrected with Scan 2523

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	62.4	16187	PASS
68	69	0.00	2	1.9	262	PASS
69	198	0.00	100	52.4	13586	PASS
70	69	0.00	2	0.3	39	PASS
127	198	10	80	57.3	14856	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	25933	PASS
199	198	5	9	6.1	1593	PASS
275	198	10	60	20.1	5207	PASS
365	198	1	100	2.6	687	PASS
441	442	0.01	24	18.1	2417	PASS
442	198	50	100	51.6	13382	PASS
443	442	15	24	19.4	2595	PASS