

Data Path : Z:\HPCHEM1\BNA E\DATA\BE121917\
 Data File : BE095037.D
 Acq On : 19 Dec 2017 17:59
 Operator : SJ/JU
 Sample : I6943-10
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Dec 20 00:49:05 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE121417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 14 18:42:53 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.46	152	5812	0.40	ng	0.00
7) Naphthalene-d8	11.31	136	14130	0.40	ng	-0.02
13) Acenaphthene-d10	15.05	164	8031	0.40	ng	-0.01
19) Phenanthrene-d10	17.74	188	18785	0.40	ng	-0.03
27) Chrysene-d12	21.84	240	19130	0.40	ng	-0.03
34) Perylene-d12	24.50	264	16920	0.40	ng	-0.05
System Monitoring Compounds						
4) 2-Fluorophenol	5.94	112	1796	0.20	ng	0.00
5) Phenol-d6	7.58	99	1814	0.14	ng	0.00
8) Nitrobenzene-d5	9.65	82	6223	0.54	ng	0.00
11) 2-Methylnaphthalene-d10	12.84	152	10159	0.44	ng	-0.02
14) 2,4,6-Tribromophenol	16.50	330	965	0.52	ng	-0.03
15) 2-Fluorobiphenyl	13.68	172	17782	0.50	ng	-0.01
25) Fluoranthene-d10	19.72	212	111038	0.46	ng	-0.03
29) Terphenyl-d14	20.28	244	25048	0.70	ng	-0.03
Target Compounds						
22) Pentachlorophenol	17.40	266	20	0.086	ng	97
32) Bis(2-ethylhexyl)phthalate	21.70	149	7311	0.103	ng	# 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE121917\
Data File : BE095037.D
Acq On : 19 Dec 2017 17:59
Operator : SJ/JU
Sample : I6943-10
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Dec 20 00:49:05 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 14 18:42:53 2017
Response via : Initial Calibration

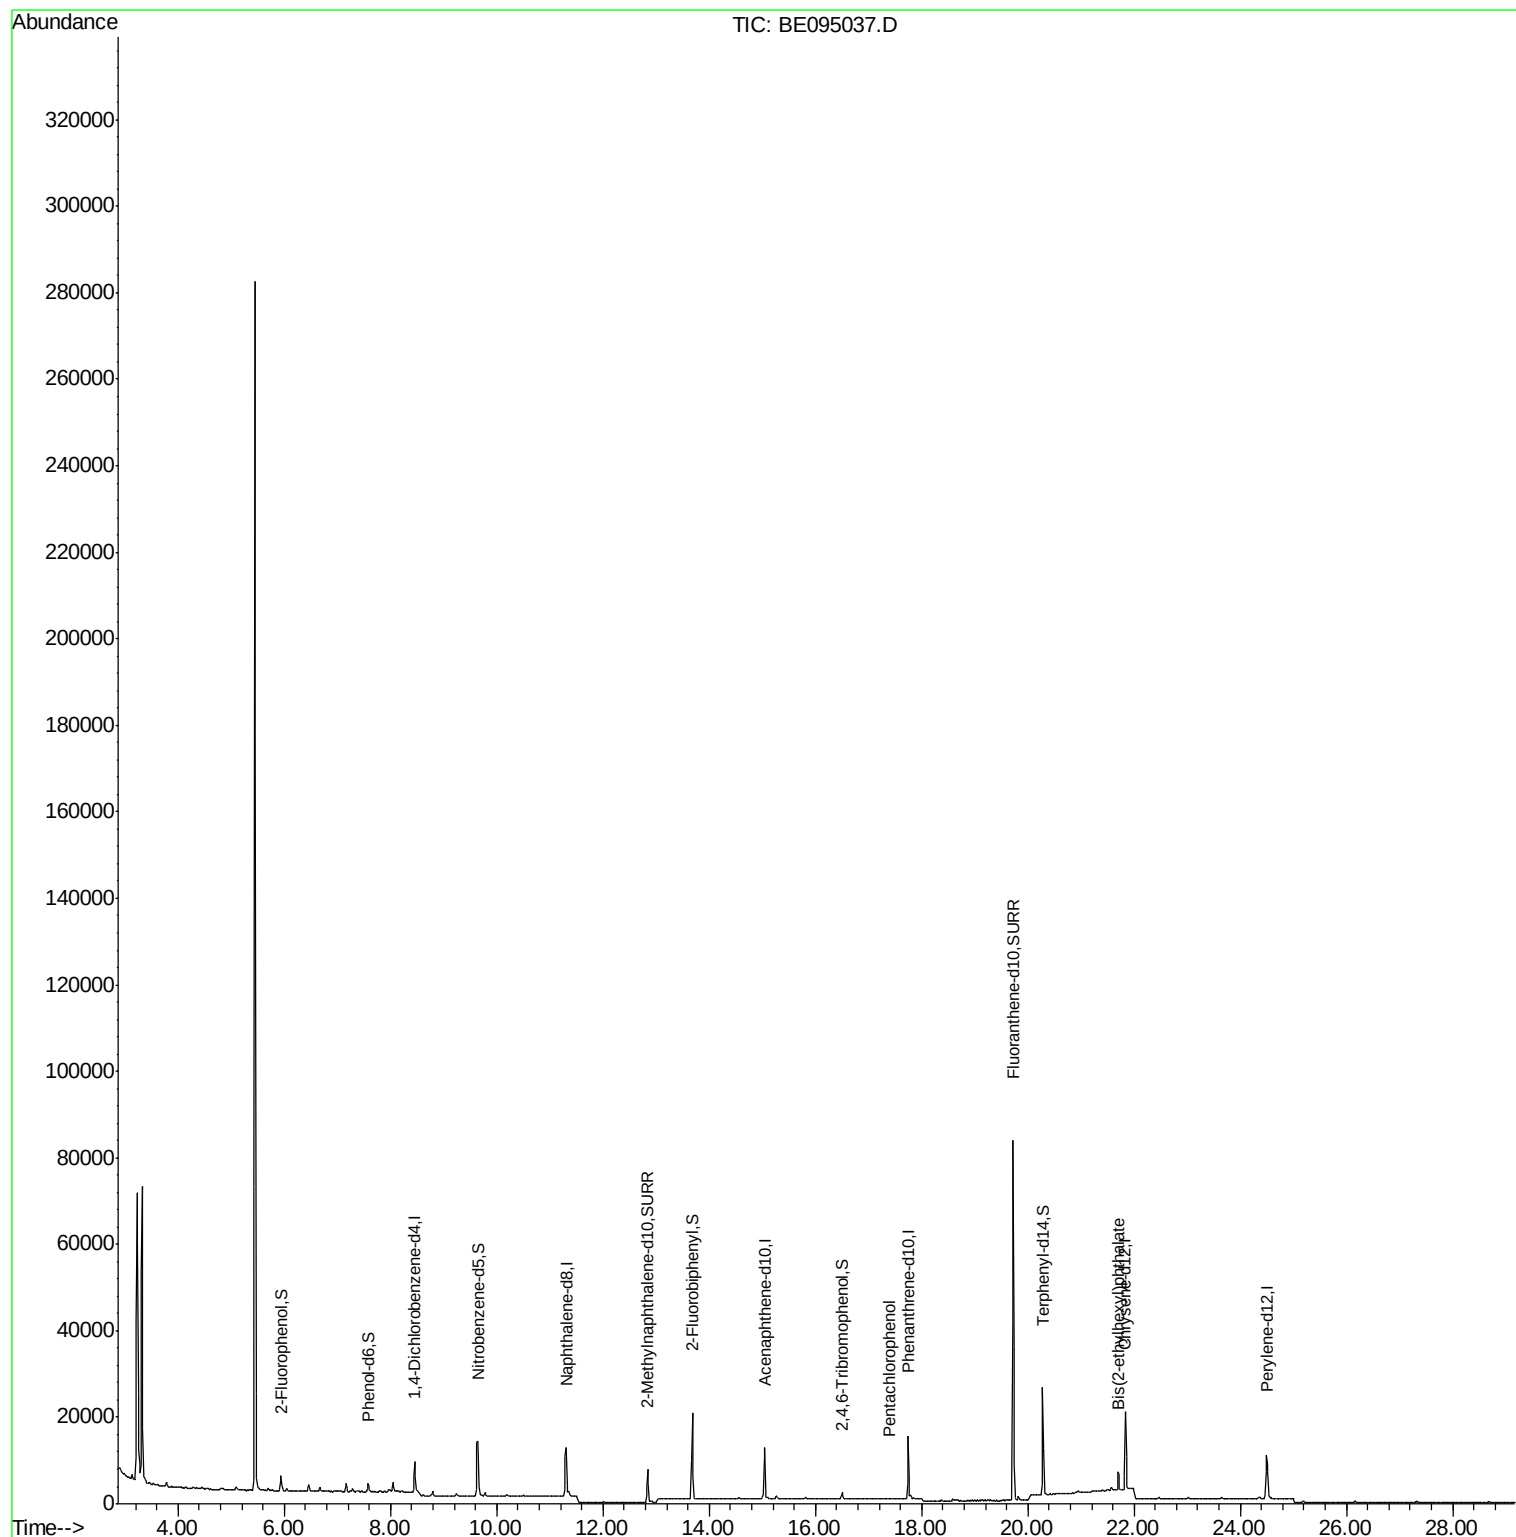




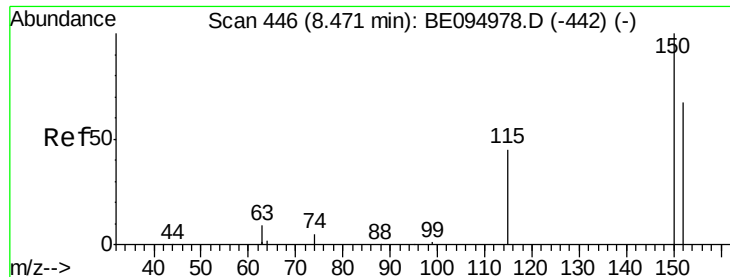


#1

1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 8.46 min Scan# 445
Delta R.T. -0.01 min
Lab File: BE095037.D
Acq: 19 Dec 2017 17:59

Instrument :
BNA_E
ClientSampleId :




Tot Ion:152 Resp: 5812
Ion Ratio Lower Upper
152 100
150 147.3 117.2 175.8
115 66.7 57.0 85.6

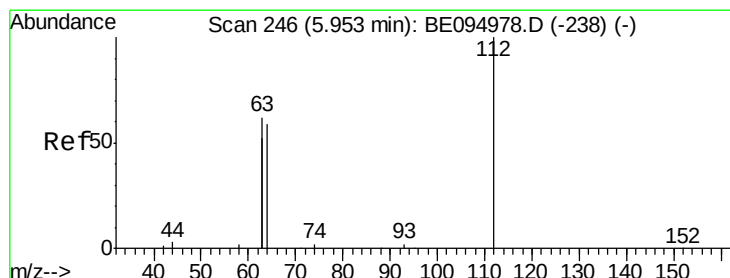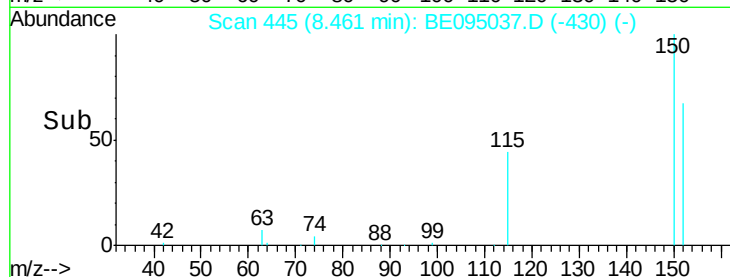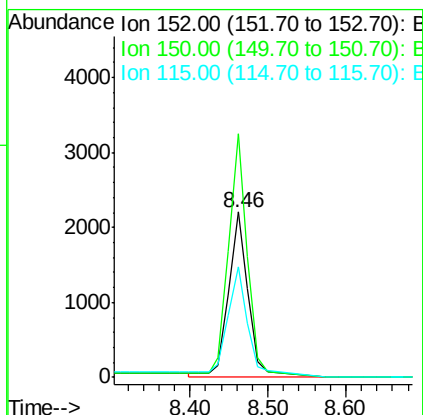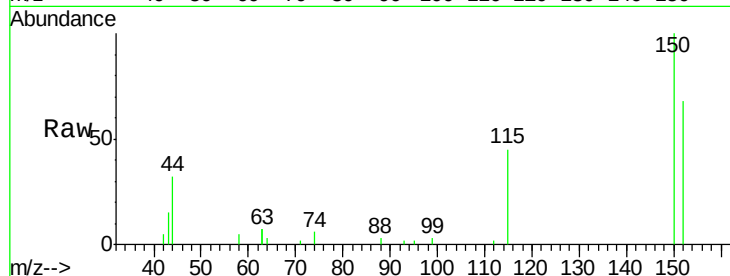


#4

2-Fluorophenol
Concen: 0.199 ng
RT: 5.94 min Scan# 245
Delta R.T. -0.01 min
Lab File: BE095037.D
Acq: 19 Dec 2017 17:59

Tgt Ion:112 Resp: 1796
Ion Ratio Lower Upper
112 100
64 71.7 60.1 90.1
63 146.6 116.8 175.2

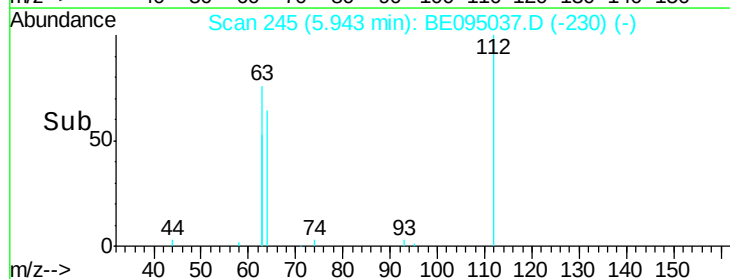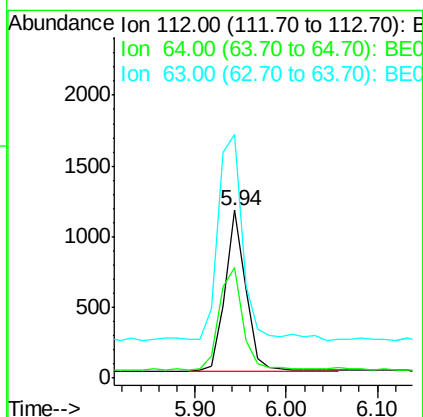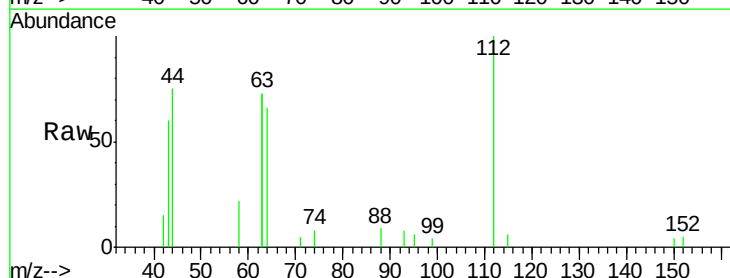

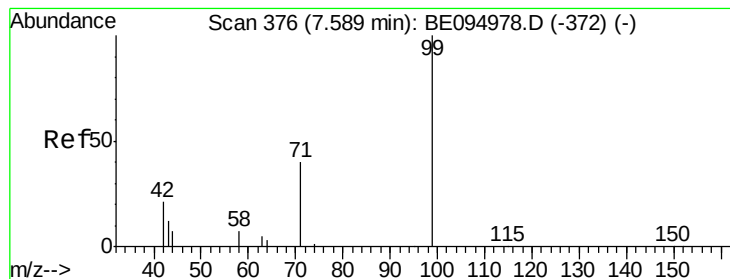

#5

Phenol-d6

Concen: 0.135 ng

RT: 7.58 min Scan# 375

Delta R.T. -0.01 min

Lab File: BE095037.D

Acq: 19 Dec 2017 17:59

Instrument :

BNA_E

ClientSampled :


Tot Ion: 99 Resp: 1814

Ion Ratio Lower Upper

99 100

42 26.2 20.2 30.2




71 40.9 28.4 42.6

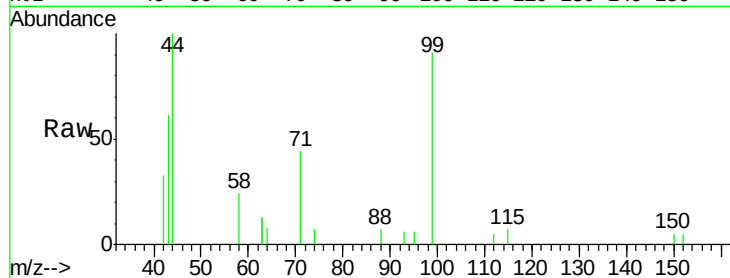

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

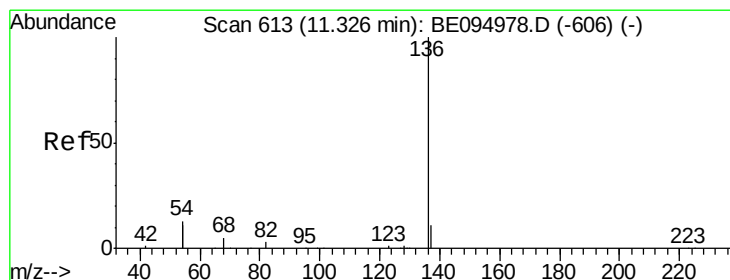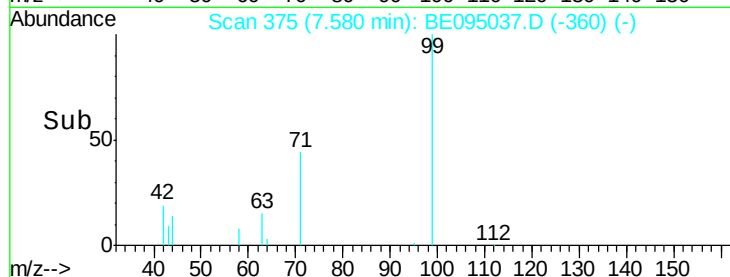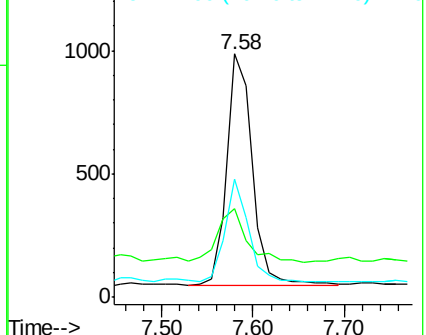

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 11.31 min Scan# 612

Delta R.T. -0.02 min

Lab File: BE095037.D

Acq: 19 Dec 2017 17:59

Tgt Ion: 136 Resp: 14130


Ion Ratio Lower Upper

136 100

137 11.6 9.5 14.3

54 22.5 29.1 43.7#

68 4.8 6.2 9.2#


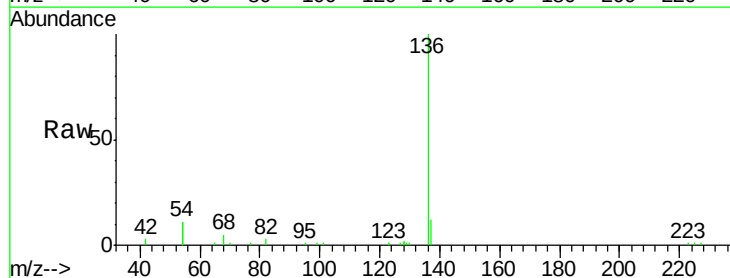



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

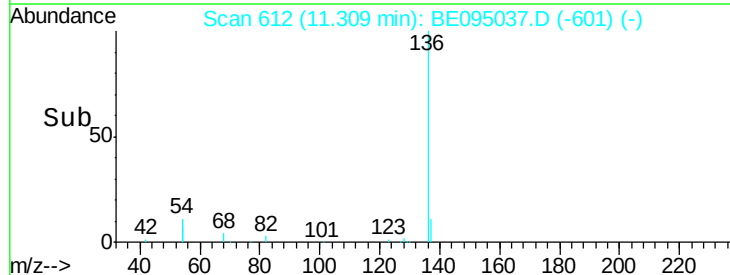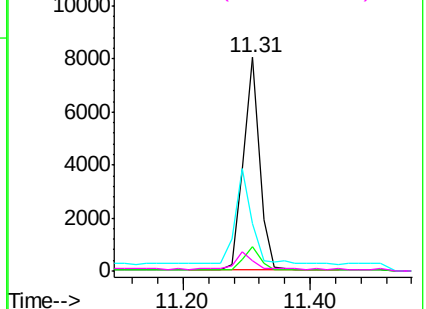



#8

Nitrobenzene-d5

Concen: 0.537 ng

RT: 9.65 min Scan# 513

Delta R.T. -0.00 min

Lab File: BE095037.D

Acq: 19 Dec 2017 17:59

Instrument :

BNA_E

ClientSampleId :


Tot Ion: 82 Resp: 6223

Ion Ratio Lower Upper

82 100

128 159.7 150.0 225.0




54 168.7 154.2 231.4

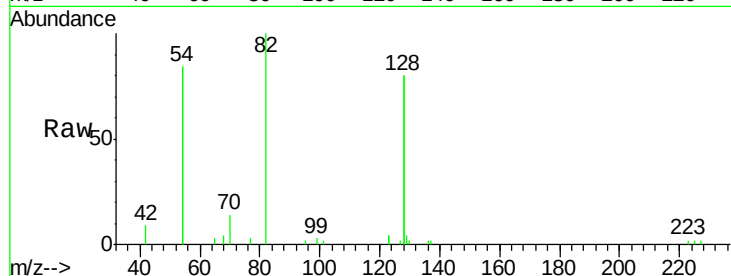

Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): BE0

Ion 54.00 (53.70 to 54.70): BE0

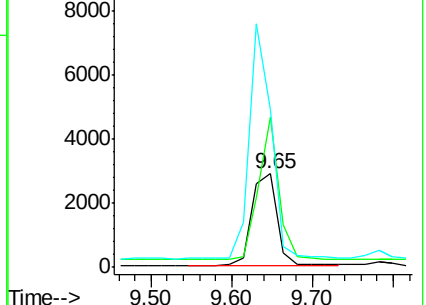

#11

2-Methylnaphthalene-d10

Concen: 0.439 ng

RT: 12.84 min Scan# 841

Delta R.T. -0.02 min

Lab File: BE095037.D


Acq: 19 Dec 2017 17:59

Tgt Ion: 152 Resp: 10159

Ion Ratio Lower Upper



152 100


151 19.5 15.4 23.0



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

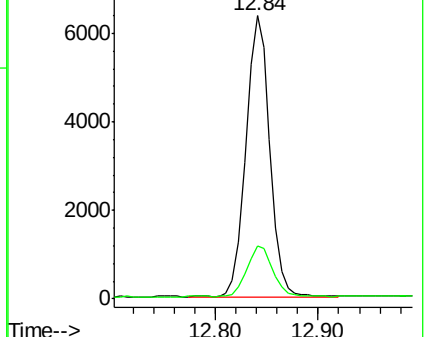



#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 15.05 min Scan# 1003

Delta R.T. -0.01 min

Lab File: BE095037.D

Acq: 19 Dec 2017 17:59

Instrument :

BNA_E

ClientSampleId :


Tot Ion:164 Resp: 8031

Ion Ratio Lower Upper

164 100

162 102.8 83.1 124.7




160 44.6 37.1 55.7

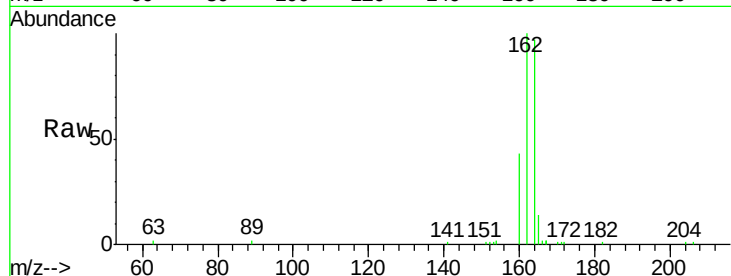

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

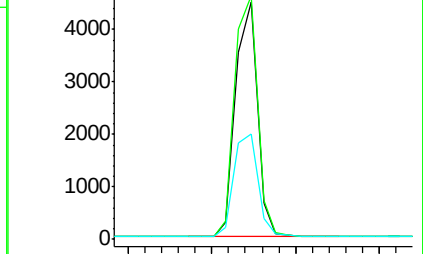

#14

2,4,6-Tribromophenol

Concen: 0.517 ng

RT: 16.50 min Scan# 1098

Delta R.T. -0.03 min

Lab File: BE095037.D

Acq: 19 Dec 2017 17:59


Tgt Ion:330 Resp: 965

Ion Ratio Lower Upper

330 100

332 95.8 152.7 229.1#



141 44.8 33.7 50.5




Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E




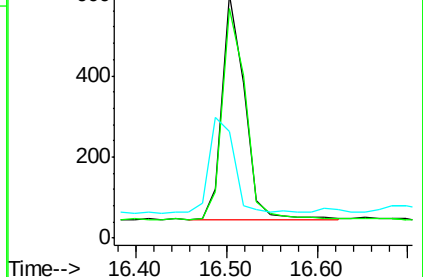


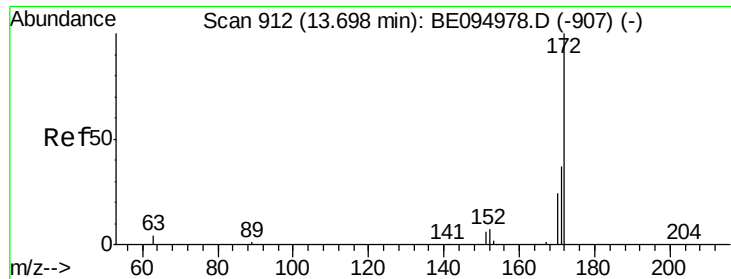

#15
2-Fluorobiphenyl
Concen: 0.500 ng
RT: 13.68 min Scan# 911
Delta R.T. -0.01 min
Lab File: BE095037.D
Acq: 19 Dec 2017 17:59




Instrument :
BNA_E
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
172	100		
171	35.6	29.9	44.9
170	22.2	21.8	32.8

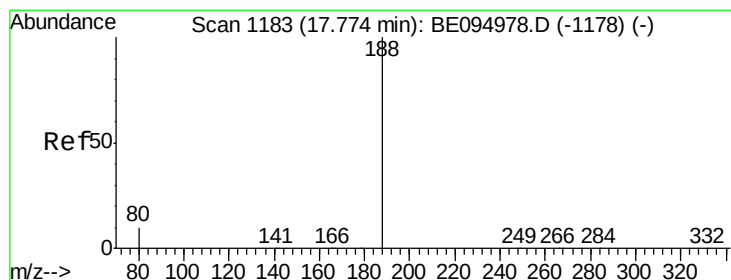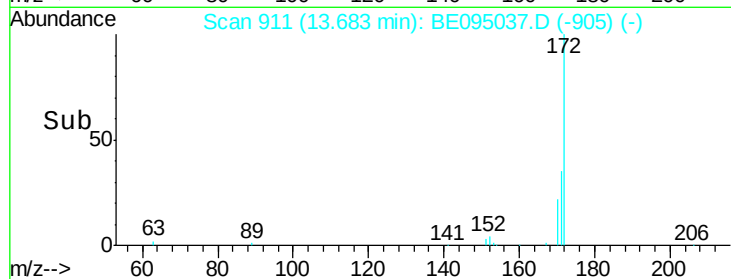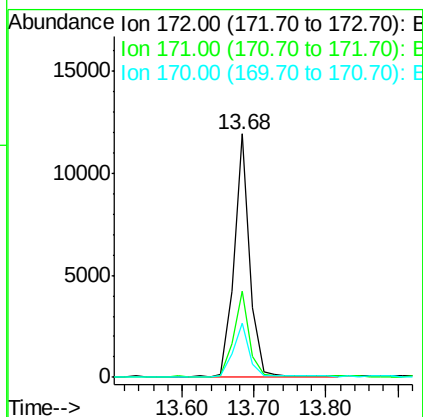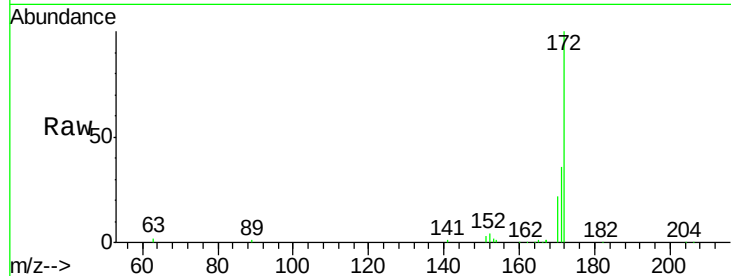

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.74 min Scan# 1181
Delta R.T. -0.03 min
Lab File: BE095037.D
Acq: 19 Dec 2017 17:59

Tgt Ion	Ratio	Lower	Upper
188	100		
94	0.0	3.9	5.9#
80	12.1	3.6	5.4#



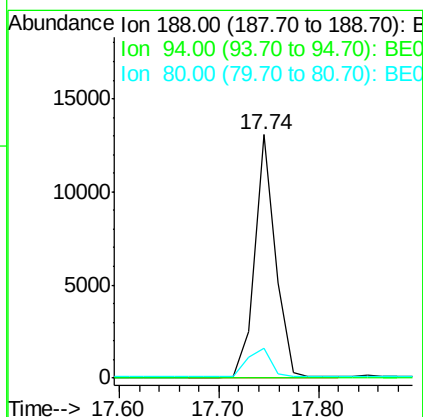



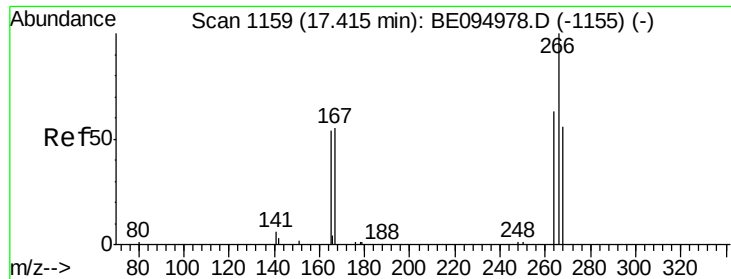

#22
 Pentachlorophenol
 Concen: 0.086 ng
 RT: 17.40 min Scan# 1158
 Delta R.T. -0.01 min
 Lab File: BE095037.D
 Acq: 19 Dec 2017 17:59




Instrument :
 BNA_E
 ClientSampleId :


Tot Ion:266 Resp: 20
 Ion Ratio Lower Upper
 266 100
 264 85.7 72.5 108.7
 268 91.1 73.8 110.6

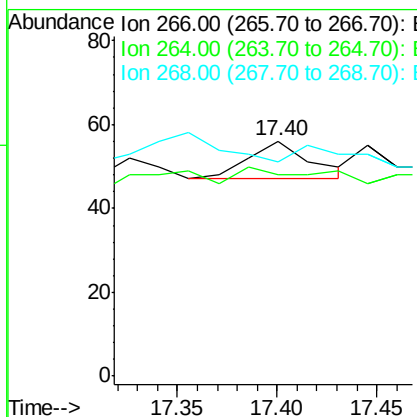

#25
 Fluoranthene-d10
 Concen: 0.456 ng
 RT: 19.72 min Scan# 1427
 Delta R.T. -0.03 min
 Lab File: BE095037.D
 Acq: 19 Dec 2017 17:59

Tgt Ion:212 Resp: 111038
 Ion Ratio Lower Upper
 212 100
 106 3.3 2.8 4.2
 104 1.9 1.6 2.4



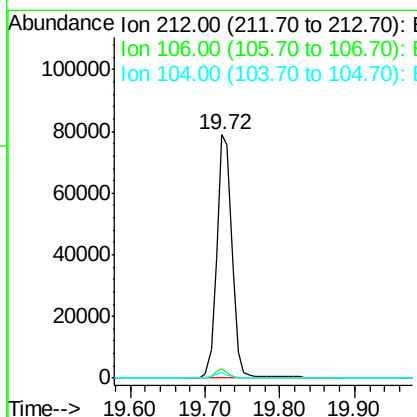





#27
 Chrysene-d12
 Concen: 0.400 ng
 RT: 21.84 min Scan# 1580
 Delta R.T. -0.03 min
 Lab File: BE095037.D
 Acq: 19 Dec 2017 17:59




Instrument :
 BNA_E
 ClientSampleId :


Tot Ion:240 Resp: 19130
 Ion Ratio Lower Upper
 240 100
 120 10.9 5.5 8.3#
 236 27.7 20.7 31.1

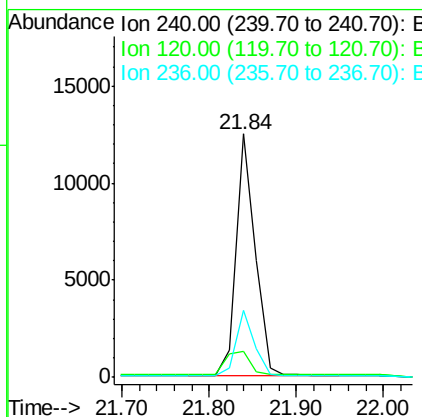

#29
 Terphenyl-d14
 Concen: 0.696 ng
 RT: 20.28 min Scan# 1480
 Delta R.T. -0.03 min
 Lab File: BE095037.D
 Acq: 19 Dec 2017 17:59

Tgt Ion:244 Resp: 25048
 Ion Ratio Lower Upper
 244 100
 212 10.5 25.4 38.0#
 122 11.8 8.1 12.1



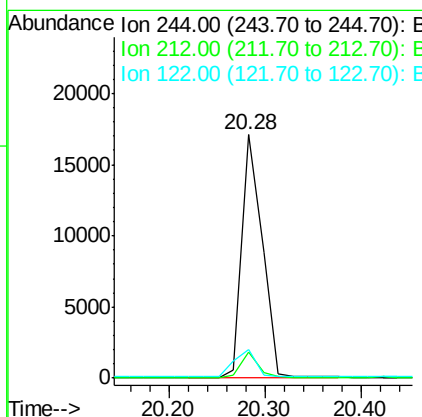





#32
 Bis(2-ethylhexyl)phthalate
 Concen: 0.103 ng
 RT: 21.70 min Scan# 1571
 Delta R.T. -0.05 min
 Lab File: BE095037.D
 Acq: 19 Dec 2017 17:59

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:149 Resp: 7311
 Ion Ratio Lower Upper
 149 100
 167 6.9 5.4 8.0
 279 1.9 0.7 1.1#

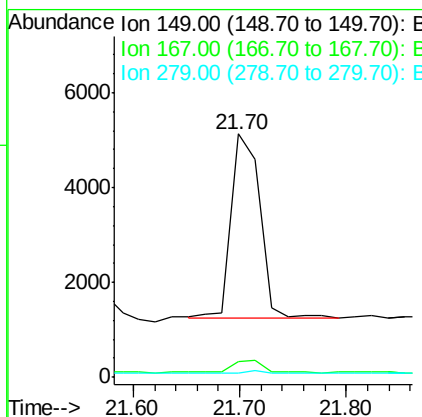

#34
 Perylene-d12
 Concen: 0.400 ng
 RT: 24.50 min Scan# 2134
 Delta R.T. -0.05 min
 Lab File: BE095037.D
 Acq: 19 Dec 2017 17:59

Tgt Ion:264 Resp: 16920
 Ion Ratio Lower Upper
 264 100
 260 24.6 20.5 30.7
 265 28.7 22.8 34.2

