
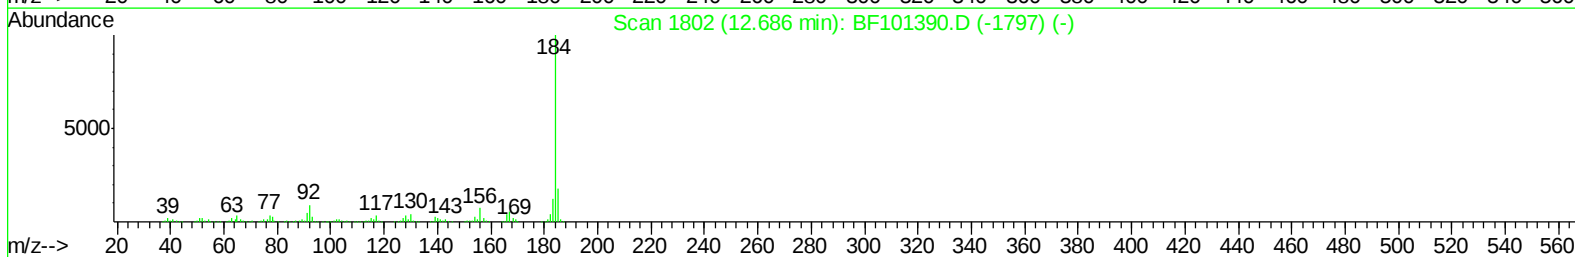
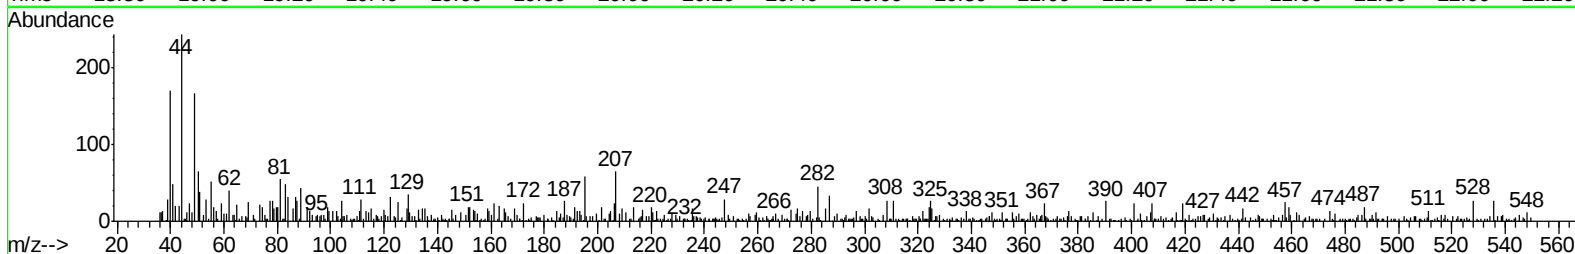


Data Path : Z:\HPCHEM1\BNA E\DATA\BE121917\
Data File : BE095027.D
Acq On : 19 Dec 2017 10:40
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 01:55:48 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 18 15:38:59 2017
Response via : Initial Calibration

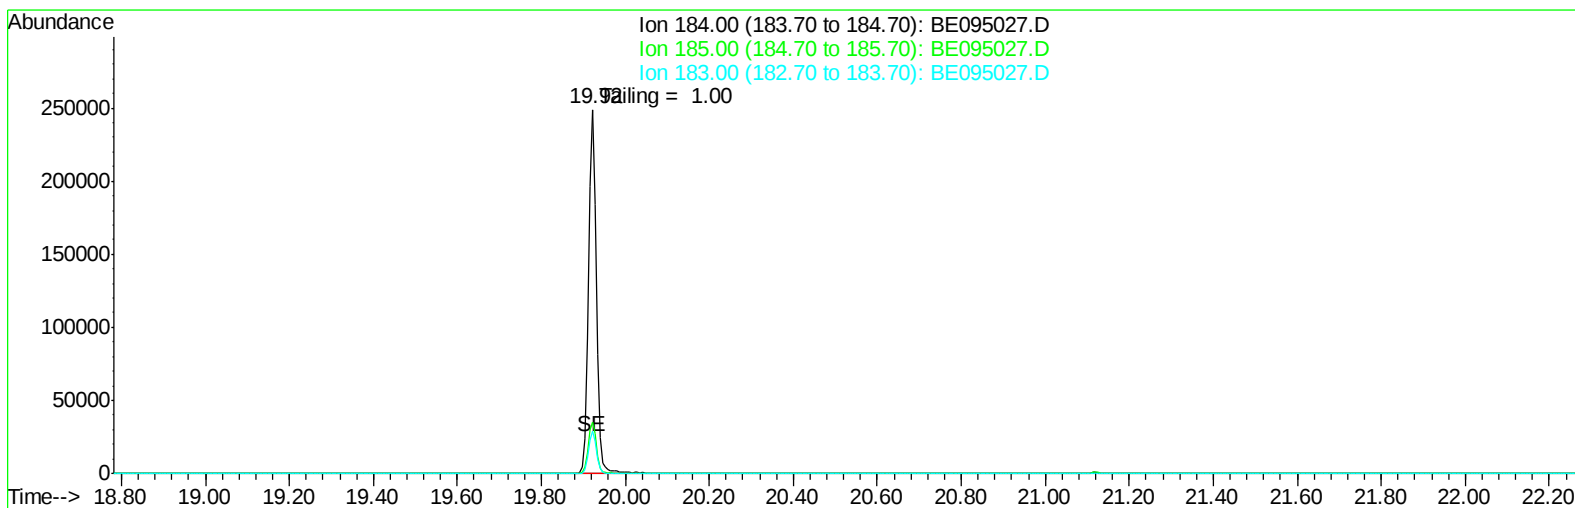

TIC: BE095027.D

(76) Benzidine




12.684min (+0.009) 16.57ng

response 7

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	38.46#
183.00	11.60	15.38#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE121917\
Data File : BE095027.D
Acq On : 19 Dec 2017 10:40
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 01:55:48 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 18 15:38:59 2017
Response via : Initial Calibration

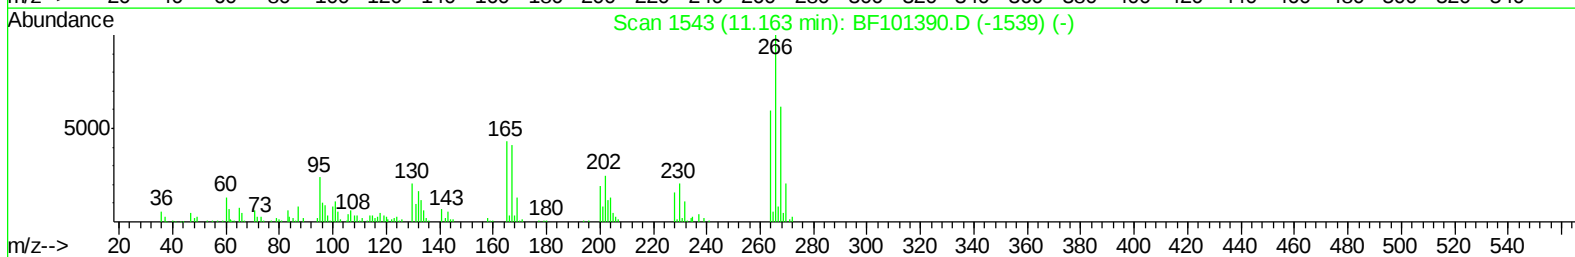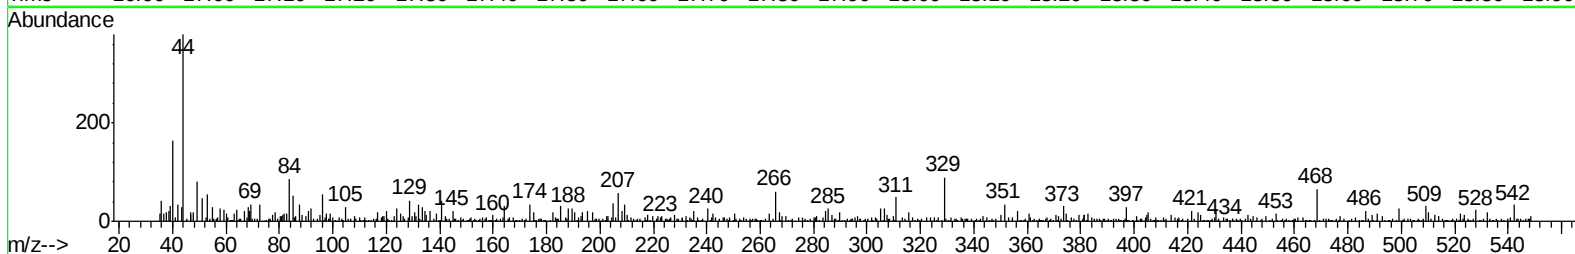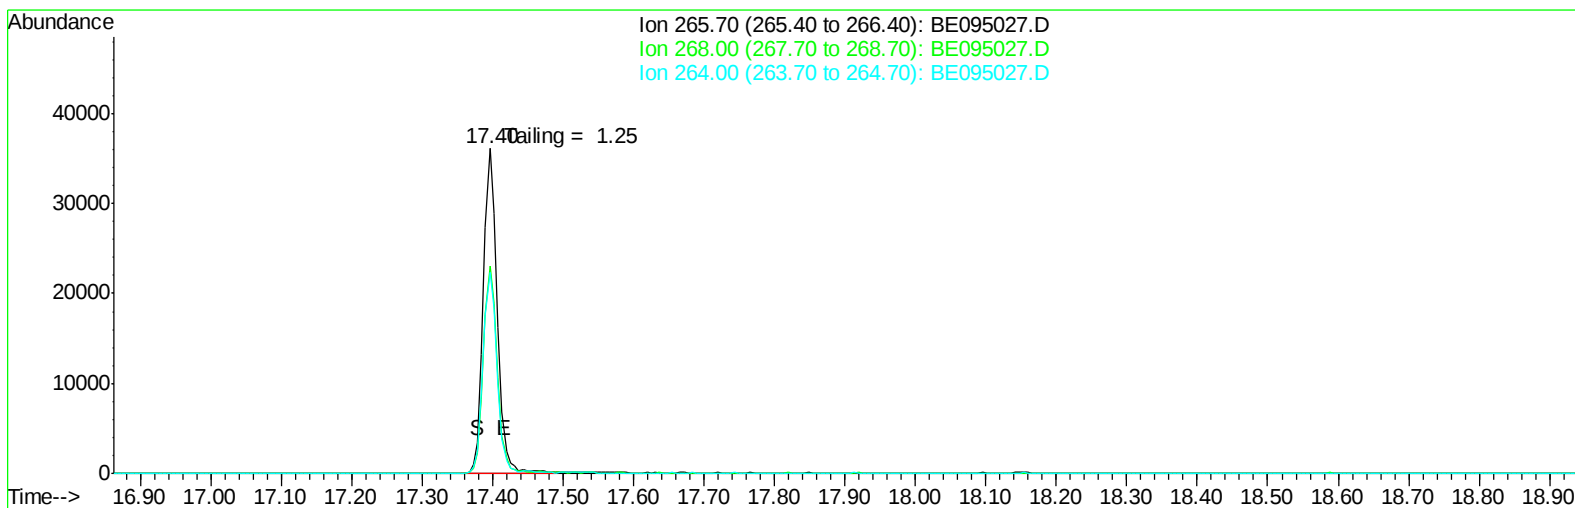

TIC: BE095027.D

(69) Pentachlorophenol (C)

11.132min (-0.018) 174.53ng

response 33

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	18.33#
264.00	61.90	8.33#
0.00	0.00	0.00