


Data Path : Z:\HPCHEM1\BNA E\DATA\BE122217\
 Data File : BE095039.D
 Acq On : 22 Dec 2017 11:03
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 14 18:42:53 2017

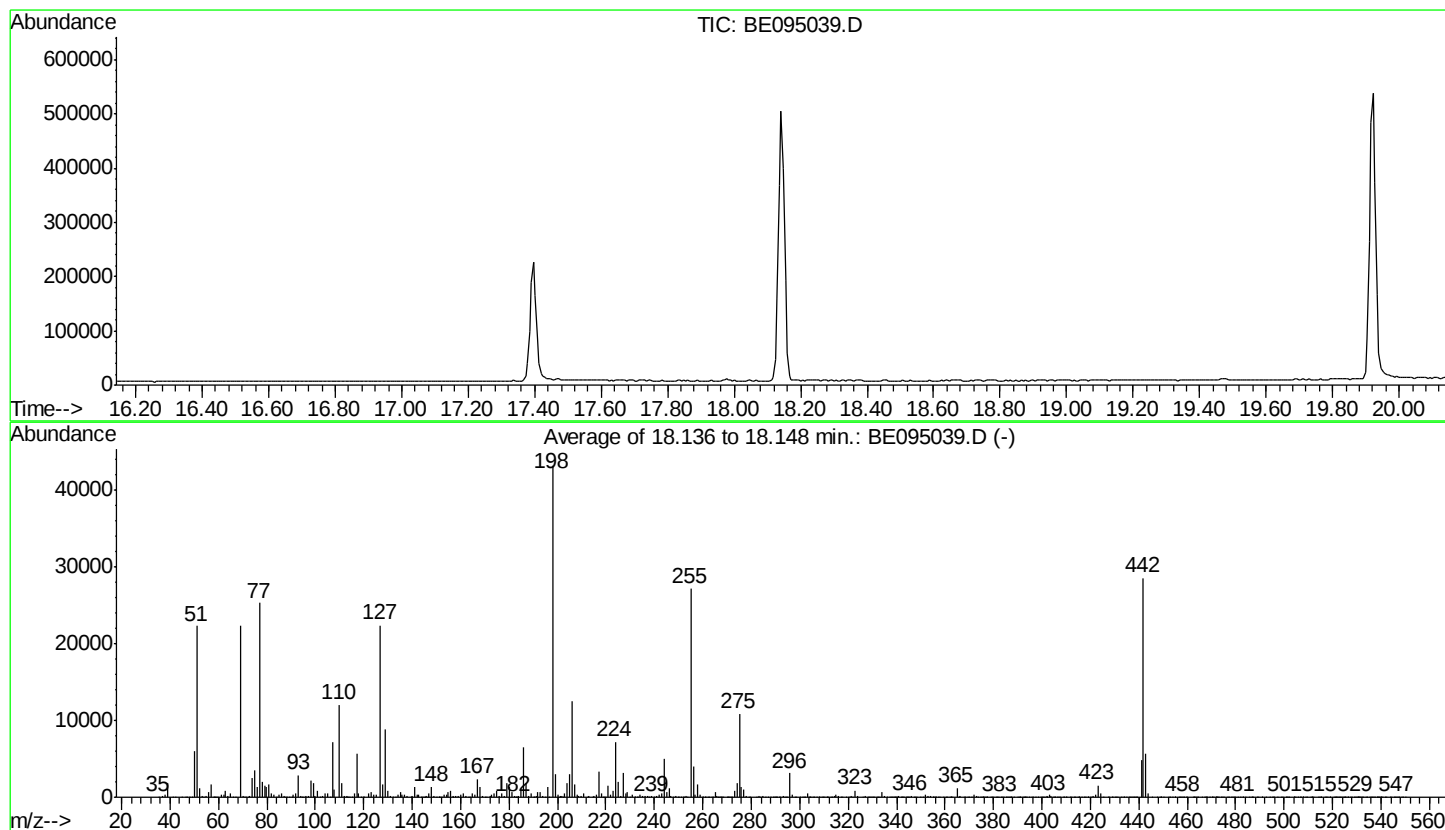

AutoFind: Scans 2646, 2647, 2648; Background Corrected with Scan 2636

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.6	22325	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	51.9	22433	PASS
70	69	0.00	2	0.6	143	PASS
127	198	10	80	51.8	22386	PASS
197	198	0.00	2	0.2	68	PASS
198	198	100	100	100.0	43250	PASS
199	198	5	9	6.8	2940	PASS
275	198	10	60	25.2	10884	PASS
365	198	1	100	2.8	1203	PASS
441	442	0.01	24	17.1	4888	PASS
442	198	50	100	66.1	28578	PASS
443	442	15	24	19.8	5655	PASS