


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE122419\
 Data File : BE100964.D
 Acq On : 24 Dec 2019 8:36
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE122419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 24 14:28:42 2019

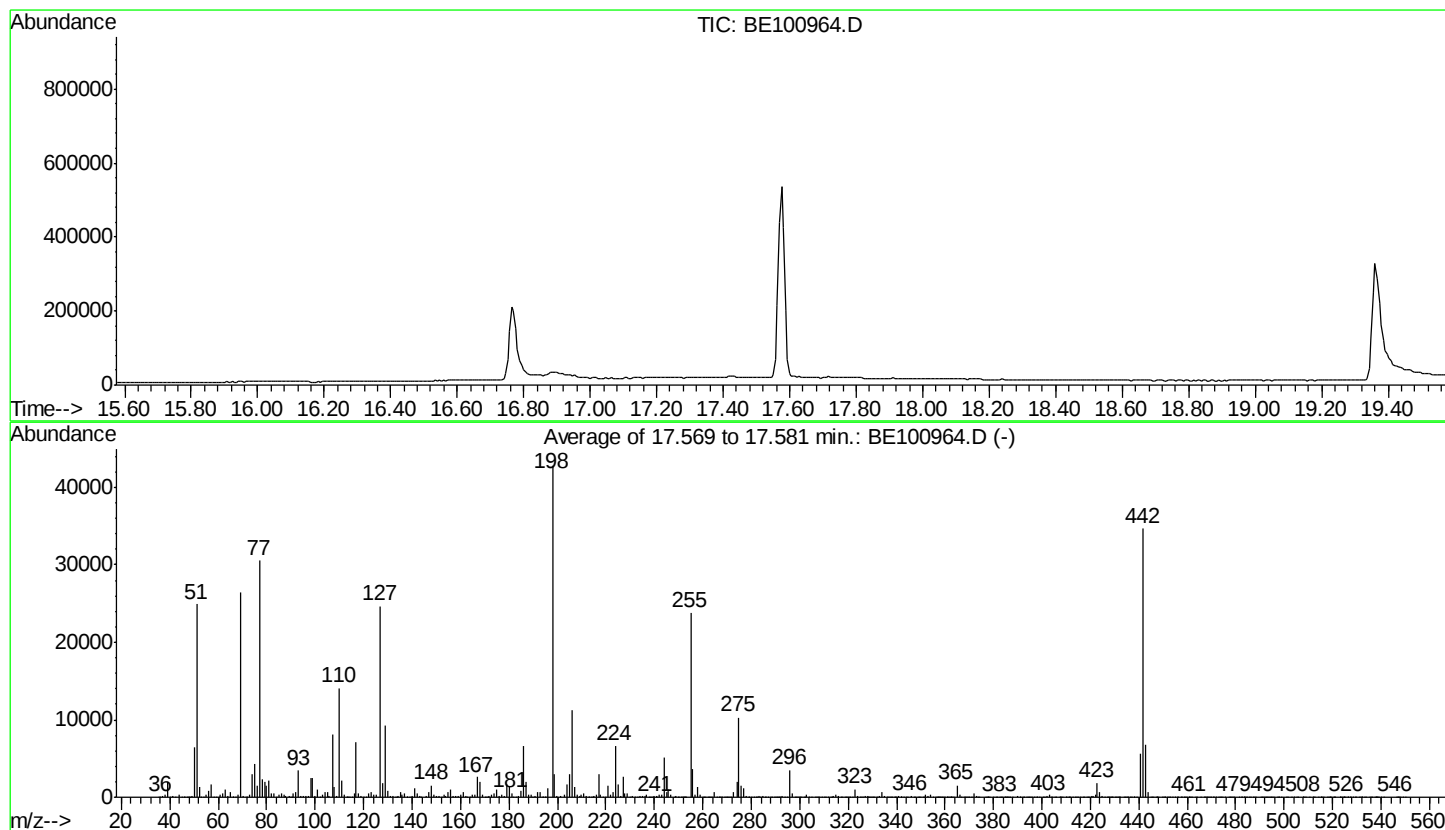

AutoFind: Scans 2550, 2551, 2552; Background Corrected with Scan 2542

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.2	24915	PASS
68	69	0.00	2	1.6	417	PASS
69	198	0.00	100	61.7	26429	PASS
70	69	0.00	2	0.5	128	PASS
127	198	10	80	57.6	24639	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	42810	PASS
199	198	5	9	7.1	3053	PASS
275	198	10	60	24.1	10322	PASS
365	198	1	100	3.6	1528	PASS
441	198	0.01	100	13.3	5691	PASS
442	198	50	100	80.9	34634	PASS
443	442	15	24	19.6	6778	PASS