
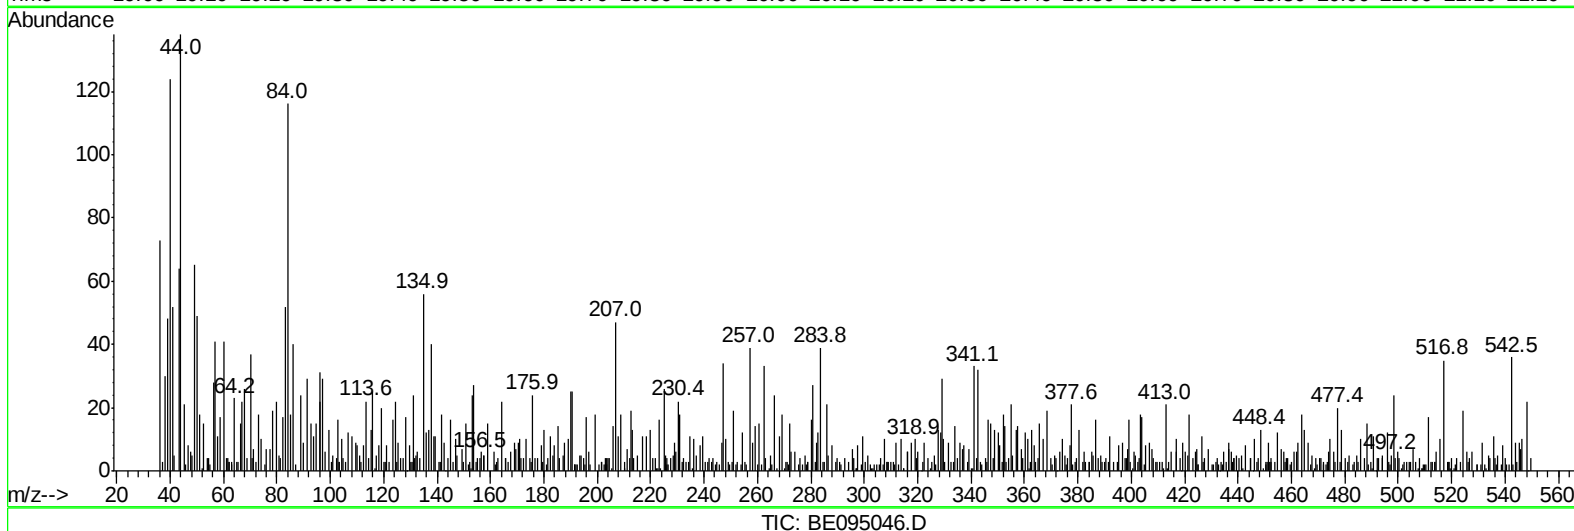


Data Path : Z:\HPCHEM1\BNA E\DATA\BE122617\
Data File : BE095046.D
Acq On : 26 Dec 2017 9:04
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 27 01:35:02 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 26 10:48:01 2017
Response via : Initial Calibration

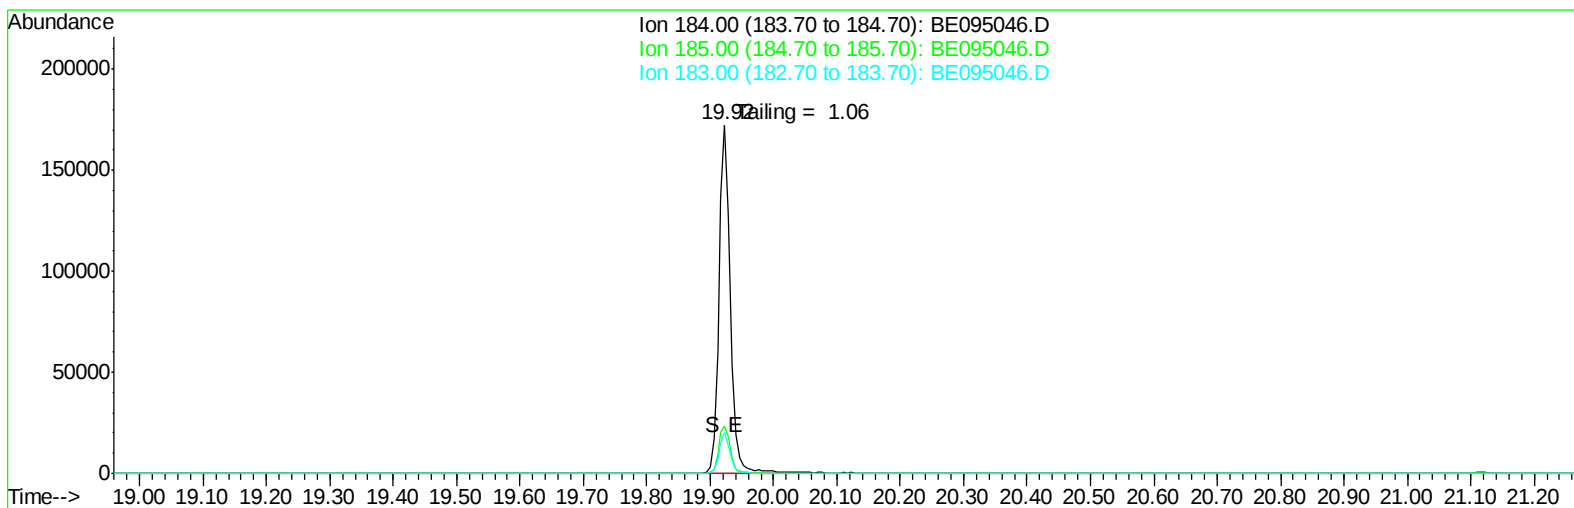

(76) Benzidine



12.861min (+0.204) 8.88ng

response 6

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	175.00#
183.00	11.60	62.50#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE122617\
Data File : BE095046.D
Acq On : 26 Dec 2017 9:04
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 27 01:35:02 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 26 10:48:01 2017
Response via : Initial Calibration

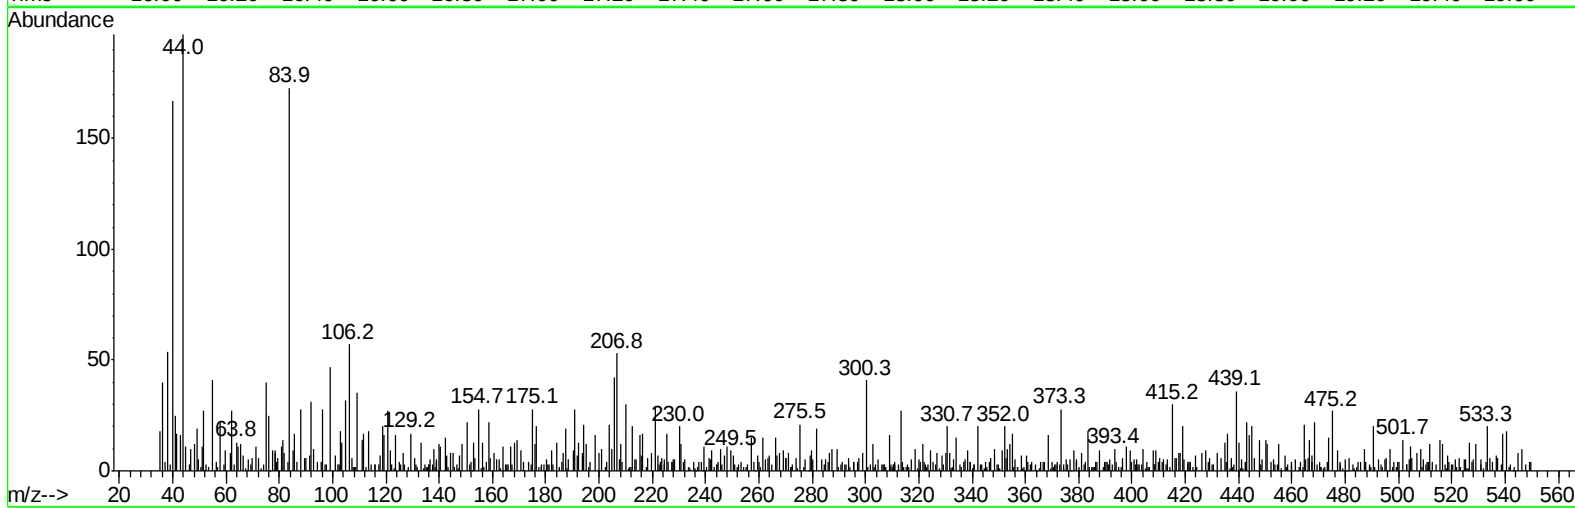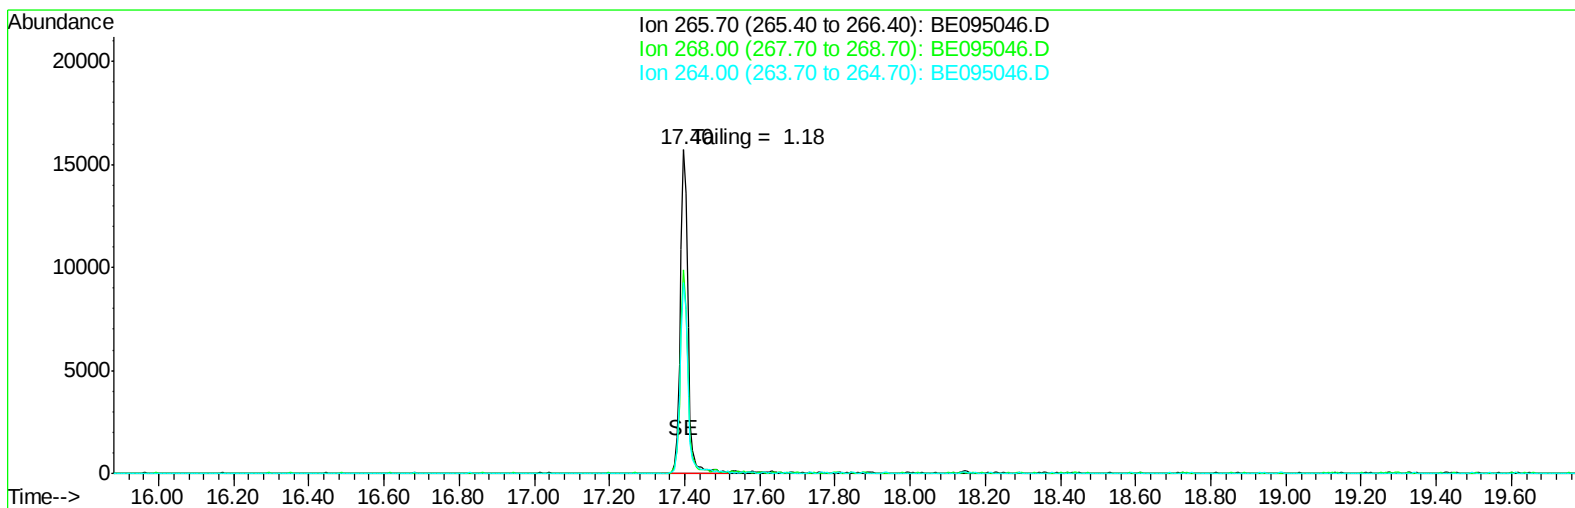

TIC: BE095046.D

(69) Pentachlorophenol (C)

10.840min (-0.299) 254.70ng

response 10

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	53.33
264.00	61.90	66.67
0.00	0.00	0.00