


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE122617\
 Data File : BE095046.D
 Acq On : 26 Dec 2017 9:04
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 27 12:15:11 2017

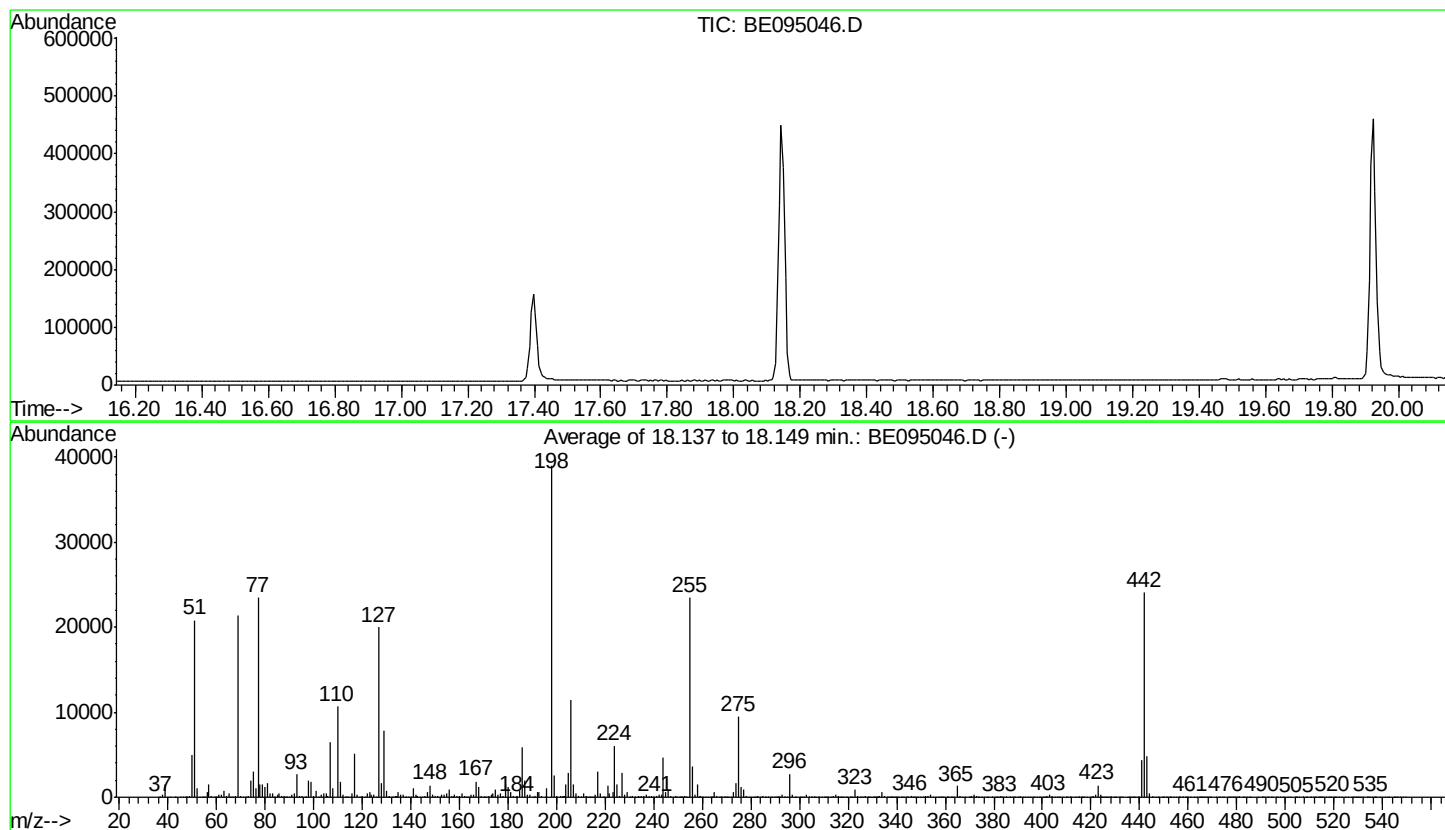

AutoFind: Scans 2646, 2647, 2648; Background Corrected with Scan 2637

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.3	20778	PASS
68	69	0.00	2	0.7	143	PASS
69	198	0.00	100	54.7	21333	PASS
70	69	0.00	2	0.6	122	PASS
127	198	10	80	51.2	19957	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	38985	PASS
199	198	5	9	6.7	2615	PASS
275	198	10	60	24.2	9450	PASS
365	198	1	100	3.3	1285	PASS
441	442	0.01	24	18.2	4364	PASS
442	198	50	100	61.6	24034	PASS
443	442	15	24	19.9	4778	PASS