
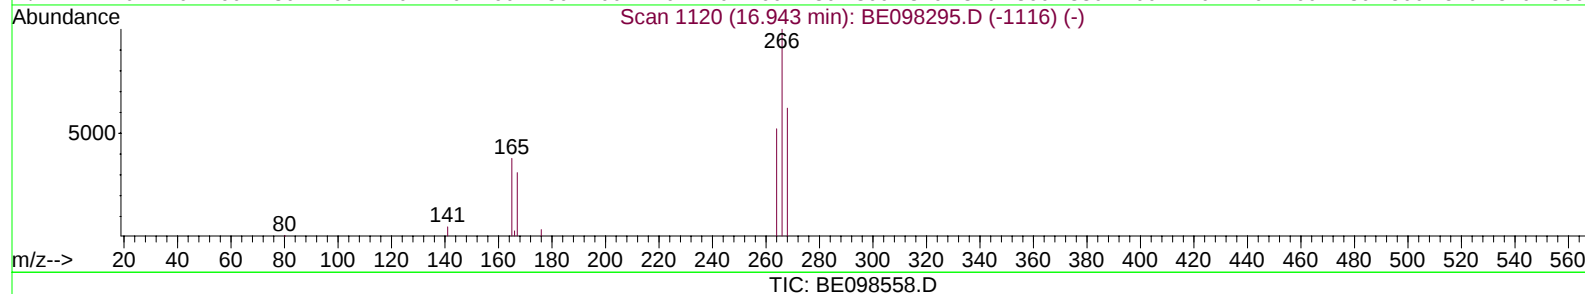
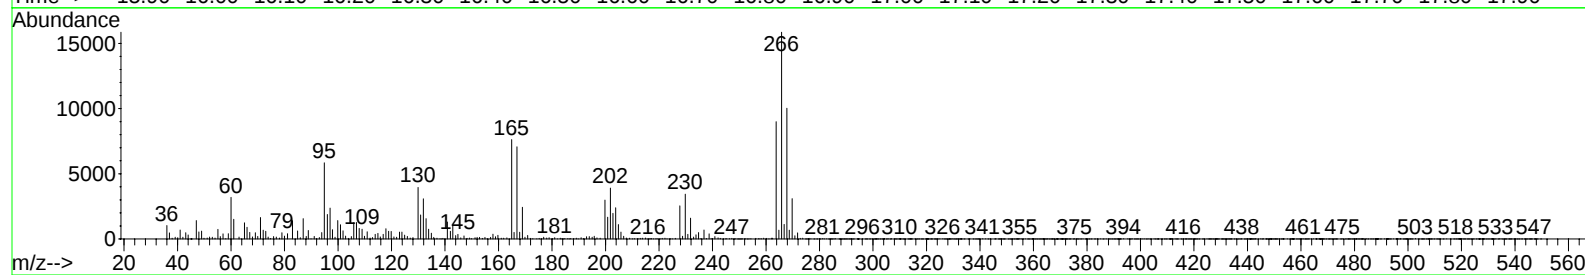


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE122618\
Data File : BE098558.D
Acq On : 26 Dec 2018 9:32
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 26 18:02:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE121018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 10 14:59:55 2018
Response via : Initial Calibration

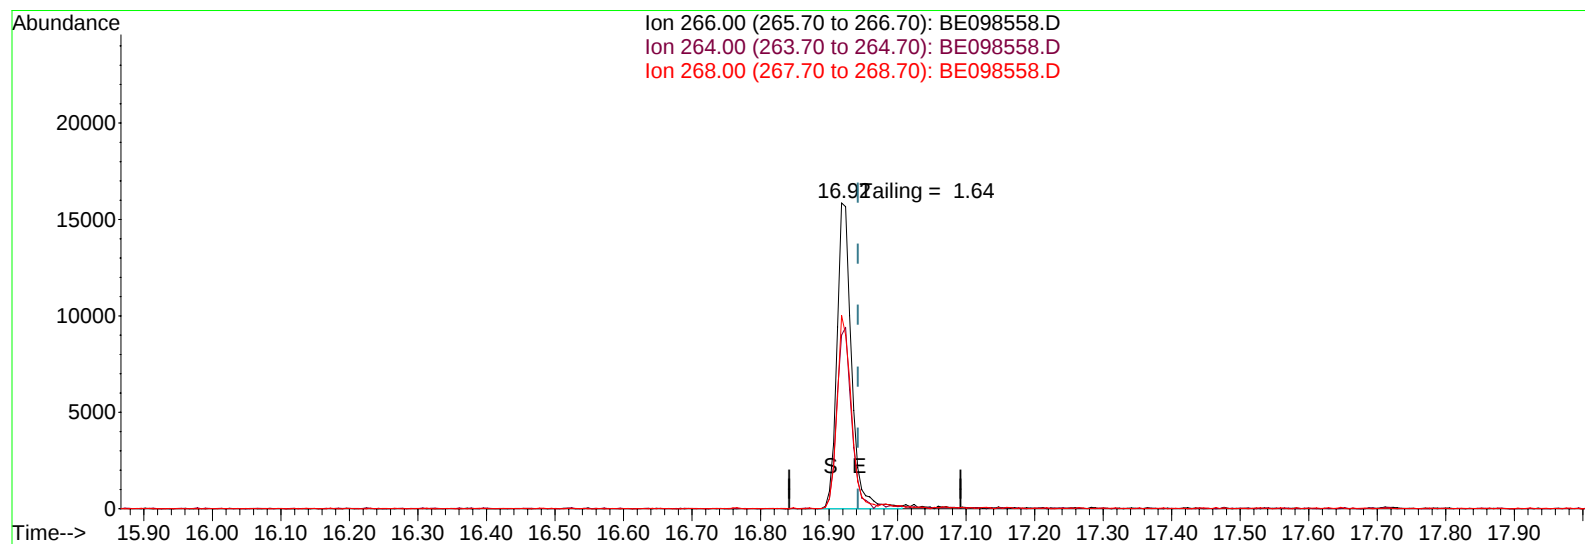

(22) Pentachlorophenol

16.918min (-0.024) 162.50ng

response 23480

Ion	Exp%	Act%
266.00	100	100
264.00	73.70	56.77#
268.00	68.90	67.47
0.00	0.00	0.00