


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE122618\
 Data File : BE098558.D
 Acq On : 26 Dec 2018 9:32
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE121018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 10 14:59:55 2018

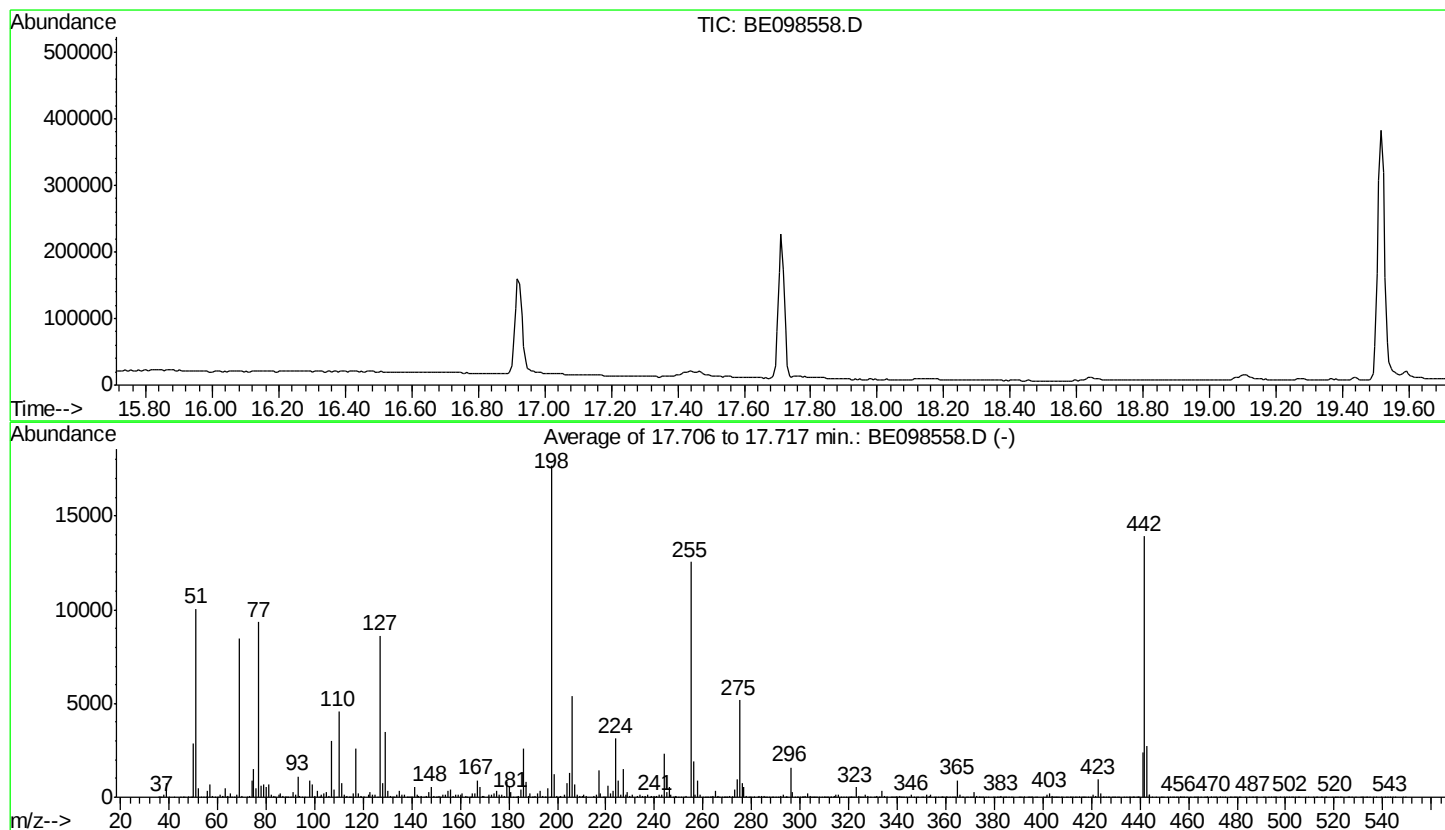

AutoFind: Scans 2573, 2574, 2575; Background Corrected with Scan 2566

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.9	10071	PASS
68	69	0.00	2	1.9	163	PASS
69	198	0.00	100	47.9	8472	PASS
70	69	0.00	2	1.0	83	PASS
127	198	10	80	48.7	8611	PASS
197	198	0.00	2	0.1	21	PASS
198	198	100	100	100.0	17693	PASS
199	198	5	9	7.0	1244	PASS
275	198	10	60	29.2	5172	PASS
365	198	1	100	5.0	889	PASS
441	198	0.01	100	13.5	2381	PASS
442	198	50	100	78.6	13914	PASS
443	442	15	24	19.5	2714	PASS