


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE122619\
 Data File : BE100973.D
 Acq On : 26 Dec 2019 15:27
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE122419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 24 14:28:42 2019

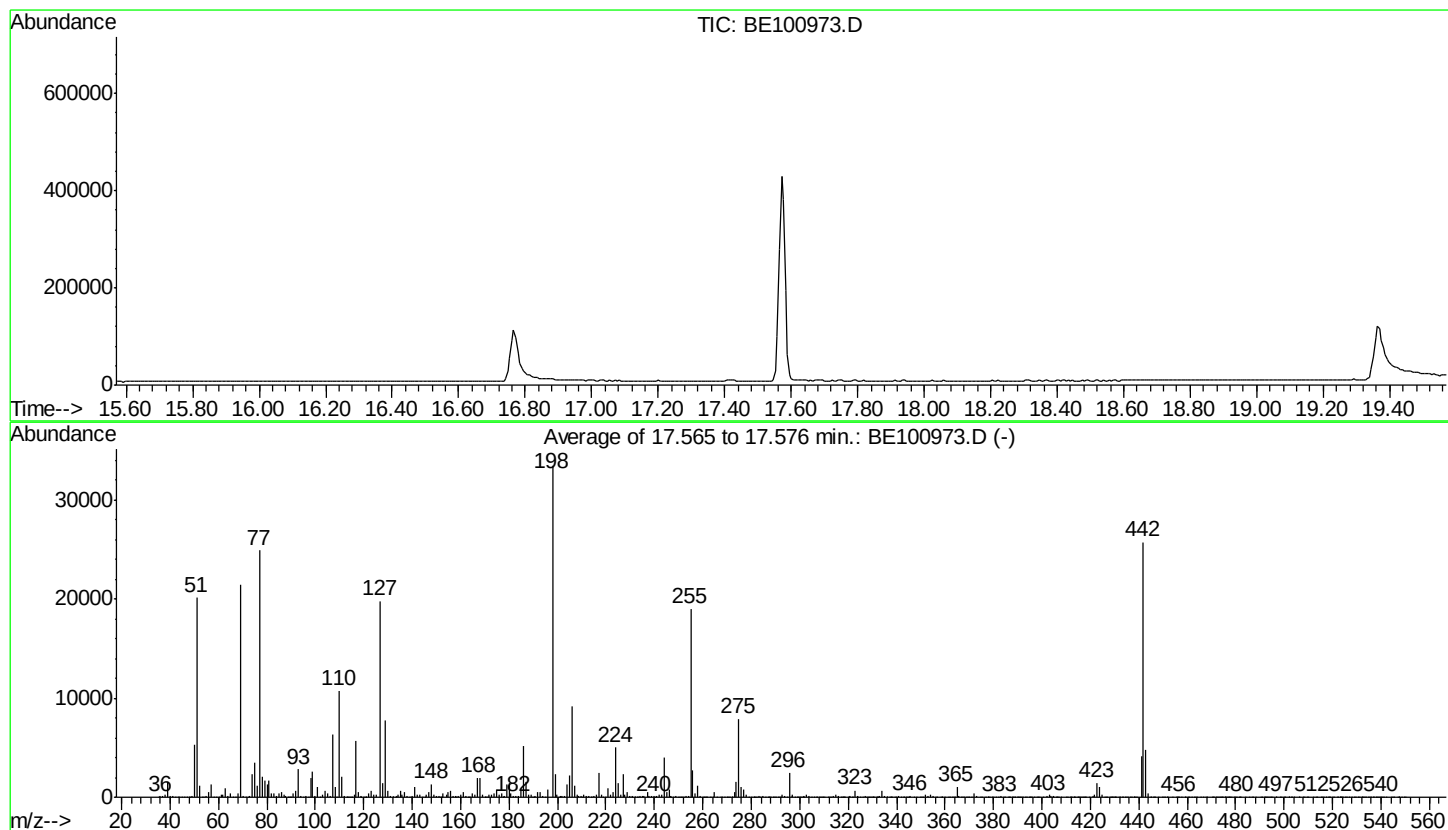

AutoFind: Scans 2549, 2550, 2551; Background Corrected with Scan 2542

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.2	20140	PASS
68	69	0.00	2	1.9	415	PASS
69	198	0.00	100	64.2	21473	PASS
70	69	0.00	2	0.5	117	PASS
127	198	10	80	59.1	19778	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	33450	PASS
199	198	5	9	6.8	2284	PASS
275	198	10	60	23.7	7932	PASS
365	198	1	100	3.2	1054	PASS
441	198	0.01	100	12.4	4132	PASS
442	198	50	100	76.9	25735	PASS
443	442	15	24	18.6	4794	PASS