


Data Path : Z:\HPCHEM1\BNA E\DATA\BE122716\
 Data File : BE092616.D
 Acq On : 27 Dec 2016 8:49
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE121916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 19 16:16:32 2016

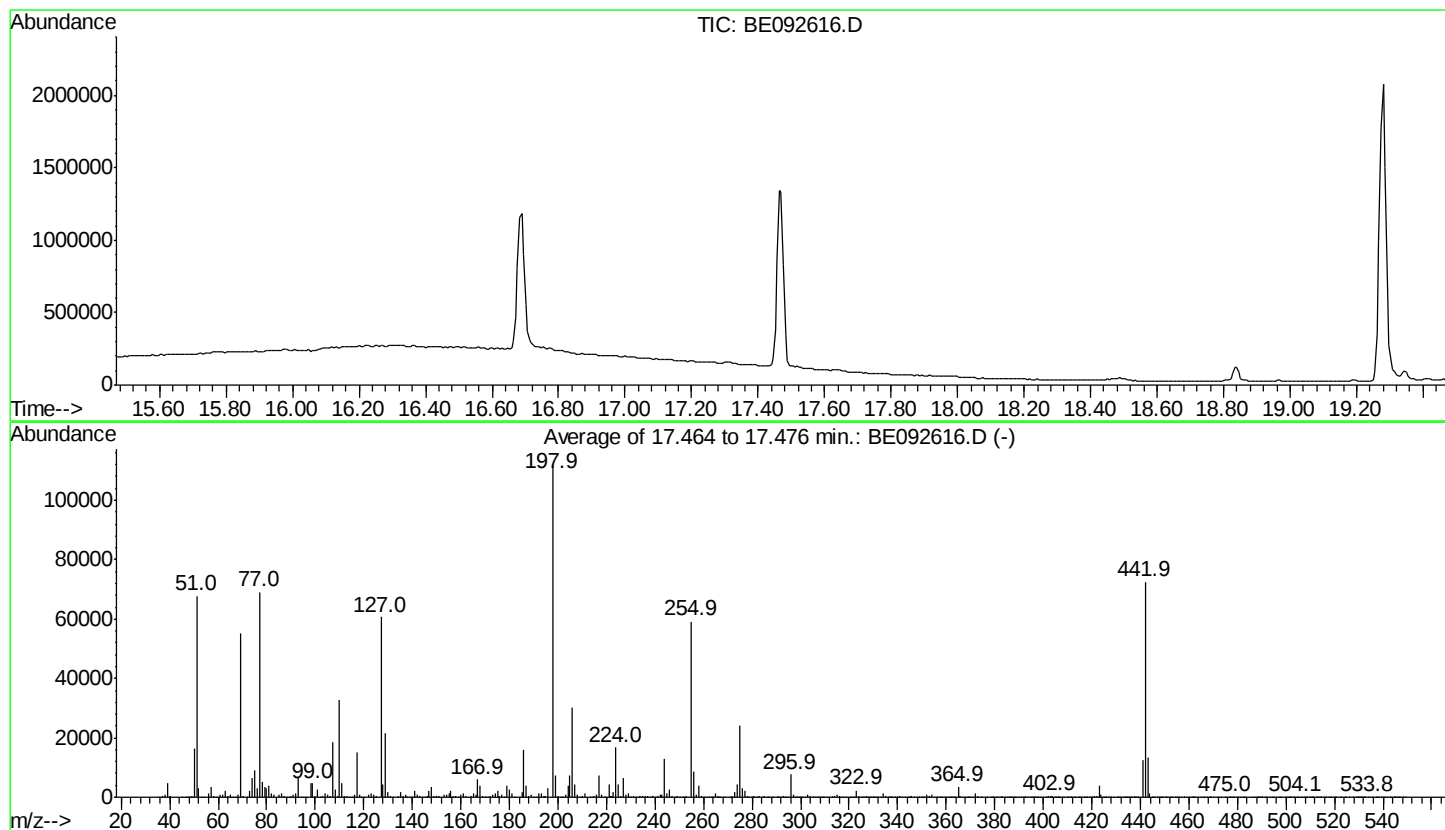

AutoFind: Scans 2532, 2533, 2534; Background Corrected with Scan 2523

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.6	67704	PASS
68	69	0.00	2	1.6	879	PASS
69	198	0.00	100	49.4	55191	PASS
70	69	0.00	2	0.4	236	PASS
127	198	10	80	54.4	60740	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	111664	PASS
199	198	5	9	6.7	7500	PASS
275	198	10	60	21.6	24130	PASS
365	198	1	100	3.1	3498	PASS
441	442	0.01	24	17.4	12606	PASS
442	198	50	100	65.0	72594	PASS
443	442	15	24	18.7	13576	PASS