
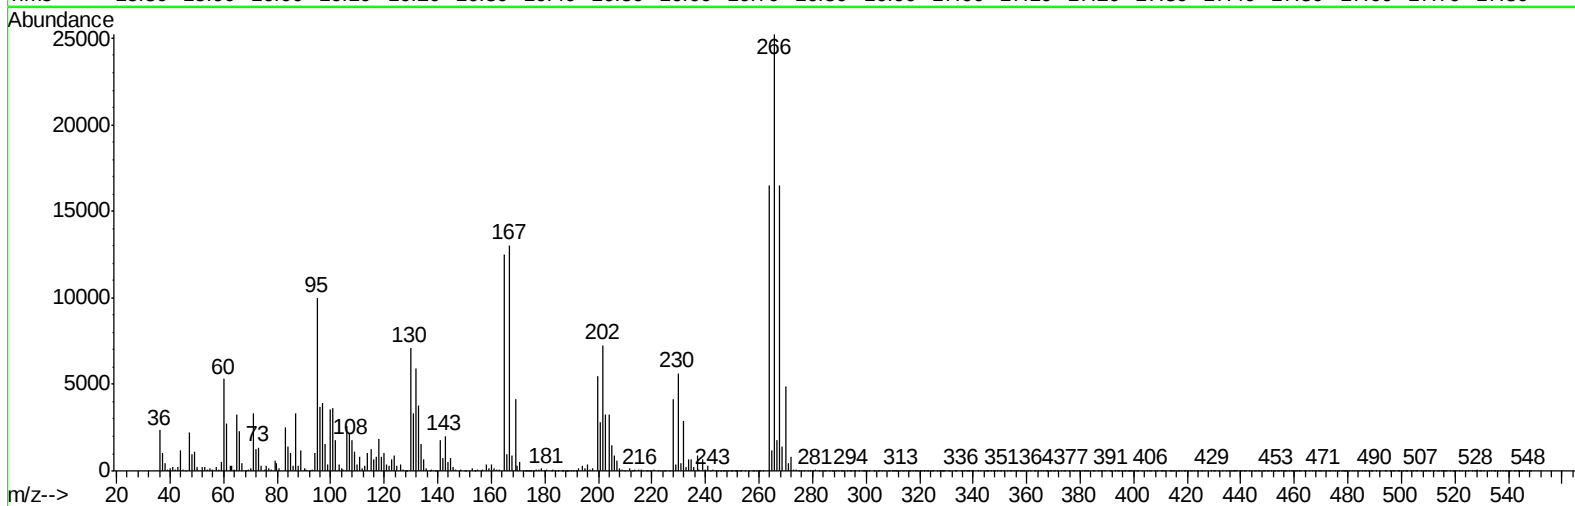


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE122719\
 Data File : BE100986.D
 Acq On : 27 Dec 2019 9:21
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 04:23:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE122419.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 27 17:39:05 2019
 Response via : Initial Calibration

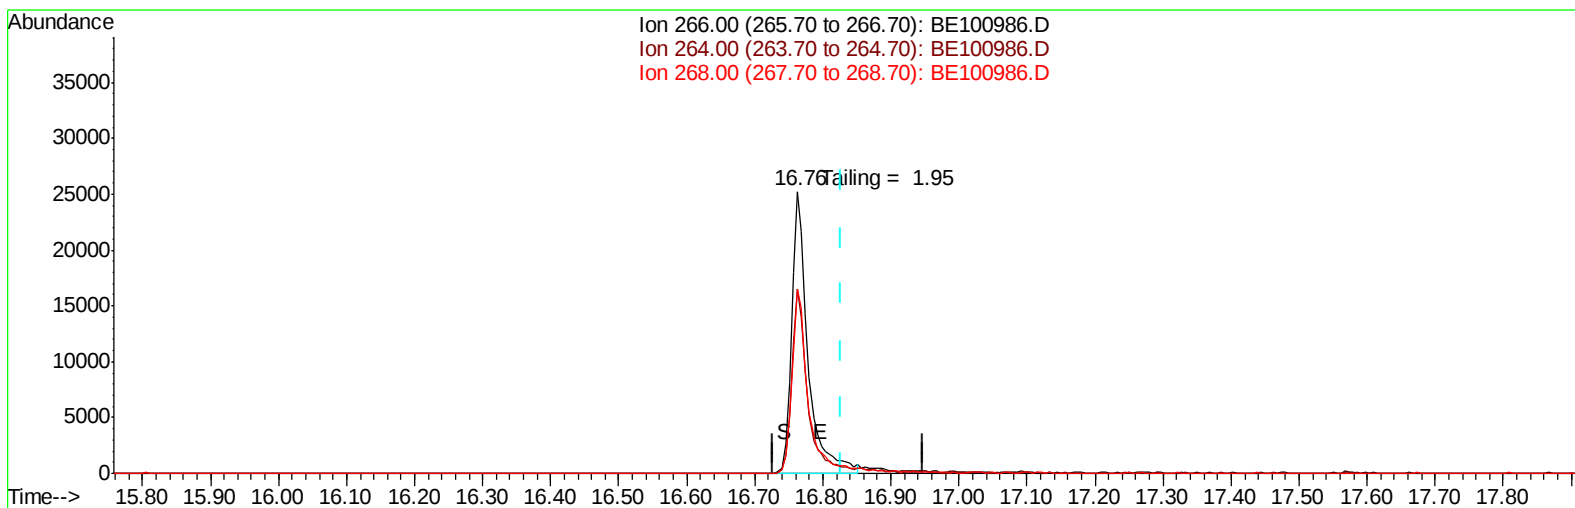

TIC: BE100986.D

(22) Pentachlorophenol

16.763min (-0.064) 234.56ng

response 31983

Ion	Exp%	Act%
266.00	100	100
264.00	77.90	65.51
268.00	82.60	65.39#
0.00	0.00	0.00