


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE122719\
 Data File : BE100986.D
 Acq On : 27 Dec 2019 9:21
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE122419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 27 17:39:05 2019

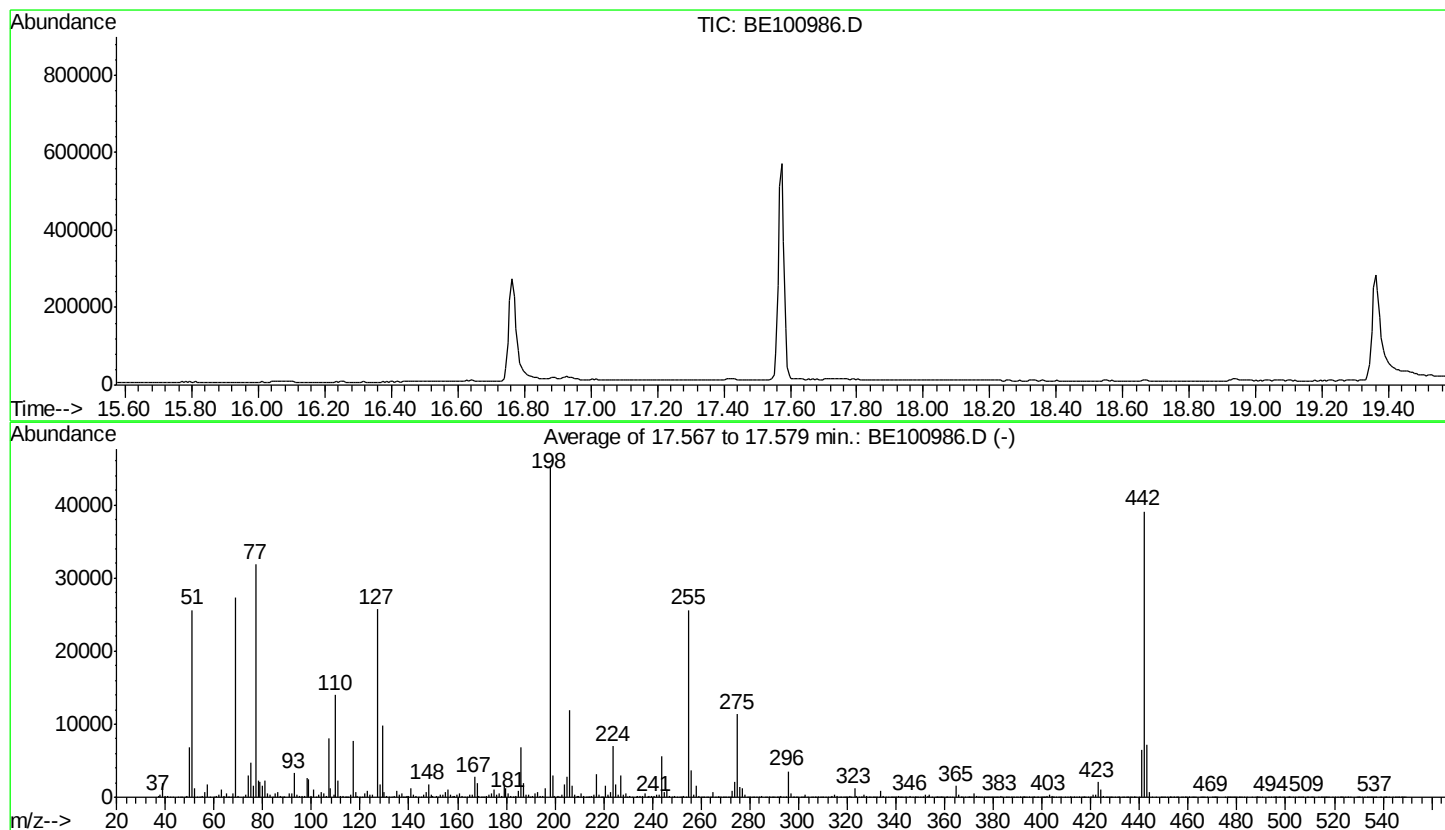

AutoFind: Scans 2549, 2550, 2551; Background Corrected with Scan 2541

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.5	25653	PASS
68	69	0.00	2	1.7	455	PASS
69	198	0.00	100	60.1	27273	PASS
70	69	0.00	2	0.4	97	PASS
127	198	10	80	56.6	25694	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	45375	PASS
199	198	5	9	6.6	2975	PASS
275	198	10	60	24.9	11321	PASS
365	198	1	100	3.5	1576	PASS
441	198	0.01	100	14.3	6481	PASS
442	198	50	100	86.2	39133	PASS
443	442	15	24	18.5	7236	PASS