


Data Path : Z:\HPCHEM1\BNA_E\Data\BE123114\
 Data File : BE089292.D
 Acq On : 31 Dec 2014 14:46
 Operator : TP/IZ
 Sample : DFTPP33
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP33

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE123014.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 31 01:01:56 2014

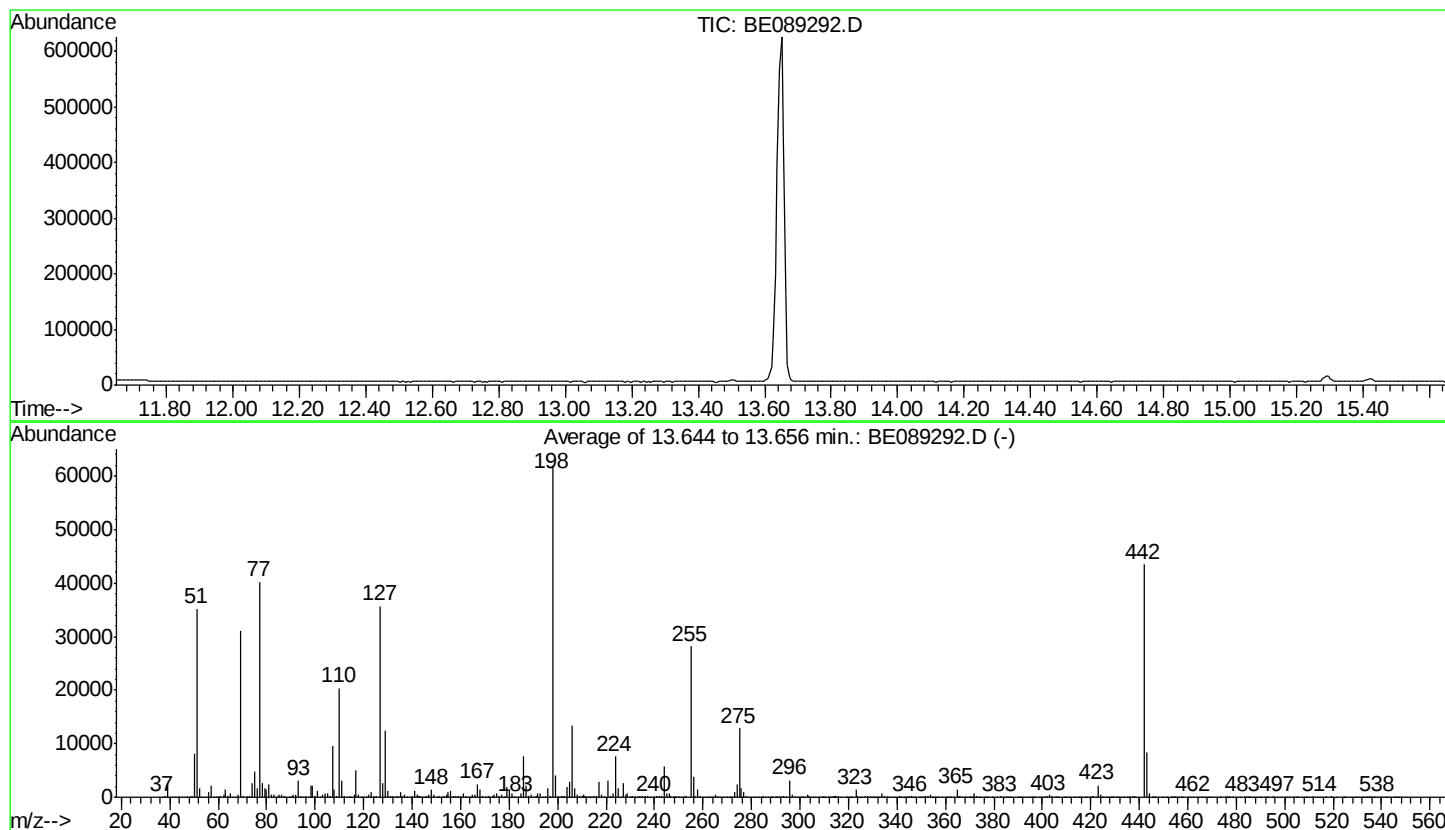

AutoFind: Scans 2086, 2087, 2088; Background Corrected with Scan 2072

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.8	35195	PASS
68	69	0.00	2	1.4	447	PASS
69	198	0.00	100	50.4	31217	PASS
70	69	0.00	2	0.6	186	PASS
127	198	10	80	57.7	35746	PASS
197	198	0.00	1	0.4	254	PASS
198	198	100	100	100.0	61969	PASS
199	198	5	9	6.7	4175	PASS
275	198	10	60	20.8	12884	PASS
365	198	1	100	2.4	1463	PASS
441	443	0.01	100	0.0	0	FAIL *
442	198	50	100	70.2	43511	PASS
443	442	15	24	19.0	8285	PASS