
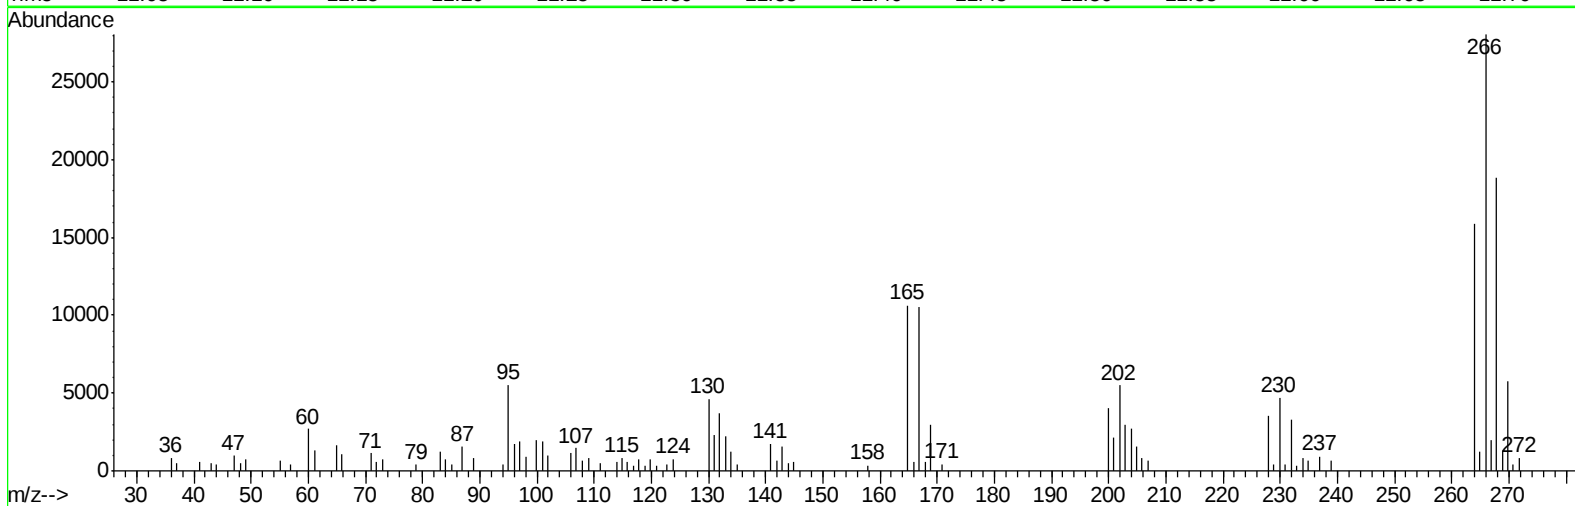


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010219\
Data File : BF111803.D
Acq On : 2 Jan 2019 11:05
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 03 05:46:08 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 17:39:39 2018
Response via : Initial Calibration

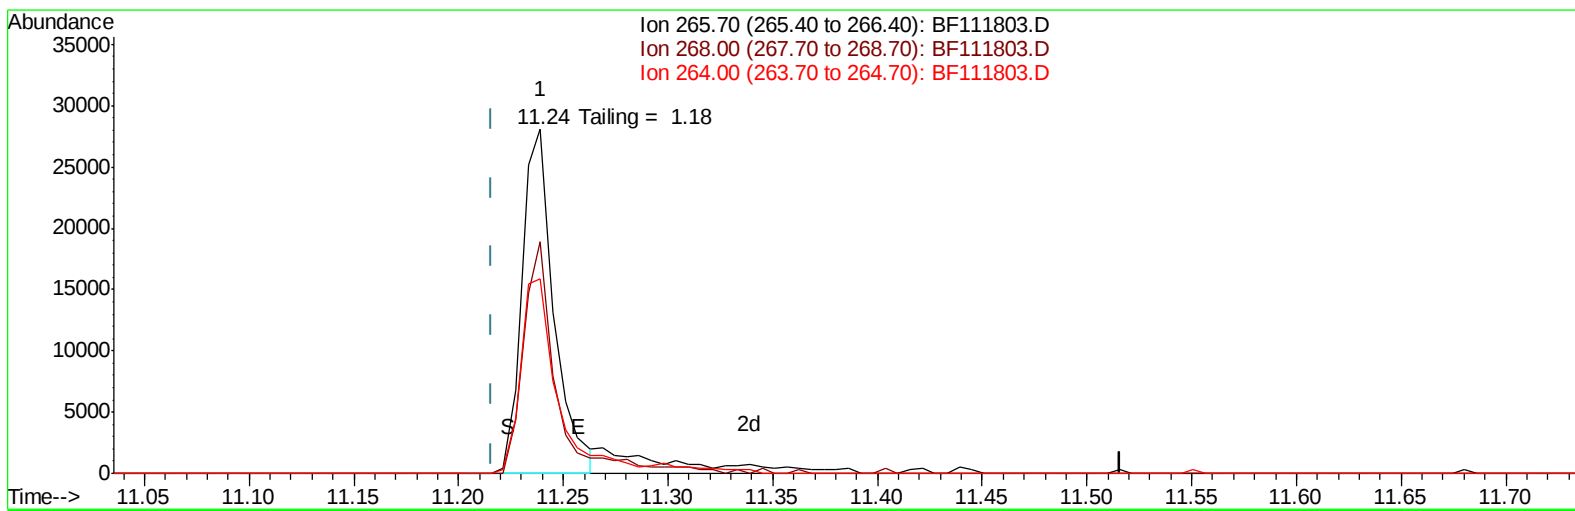

TIC: BF111803.D

(70) Pentachlorophenol (C)



11.239min (+0.023) 9475.95ng

response 33702

Ion	Exp%	Act%
265.70	100	100
268.00	59.90	67.27
264.00	61.40	56.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010219\
 Data File : BF111803.D
 Acq On : 2 Jan 2019 11:05
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 03 05:46:08 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 19 17:39:39 2018
 Response via : Initial Calibration

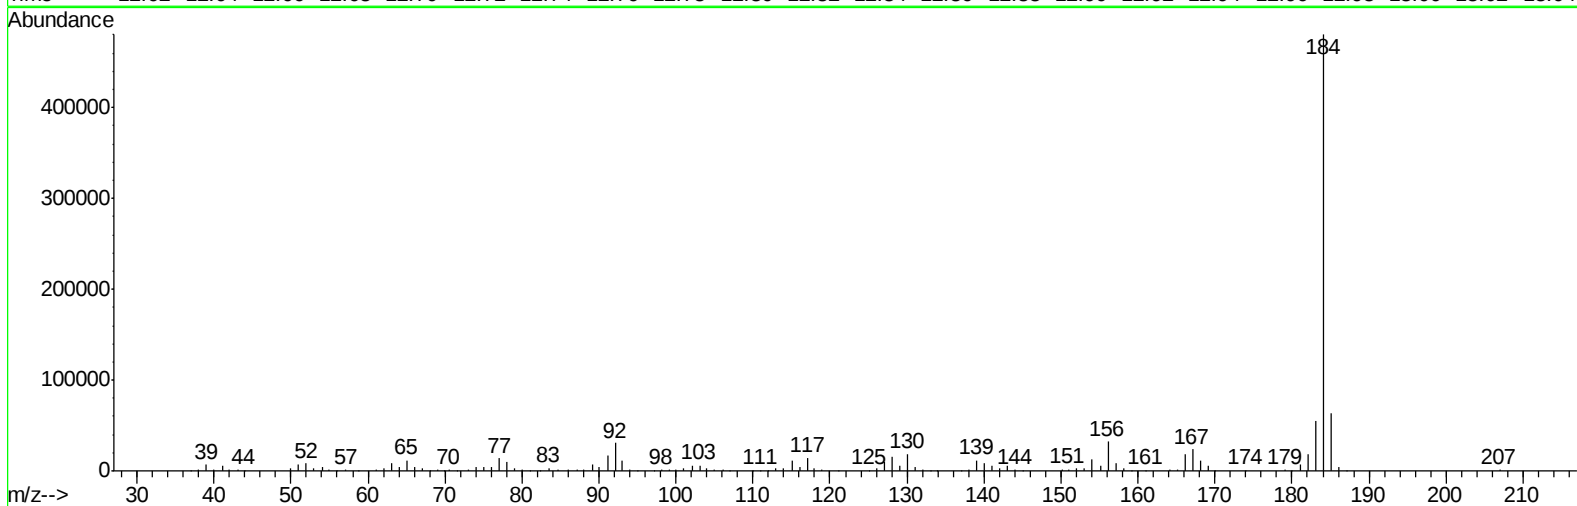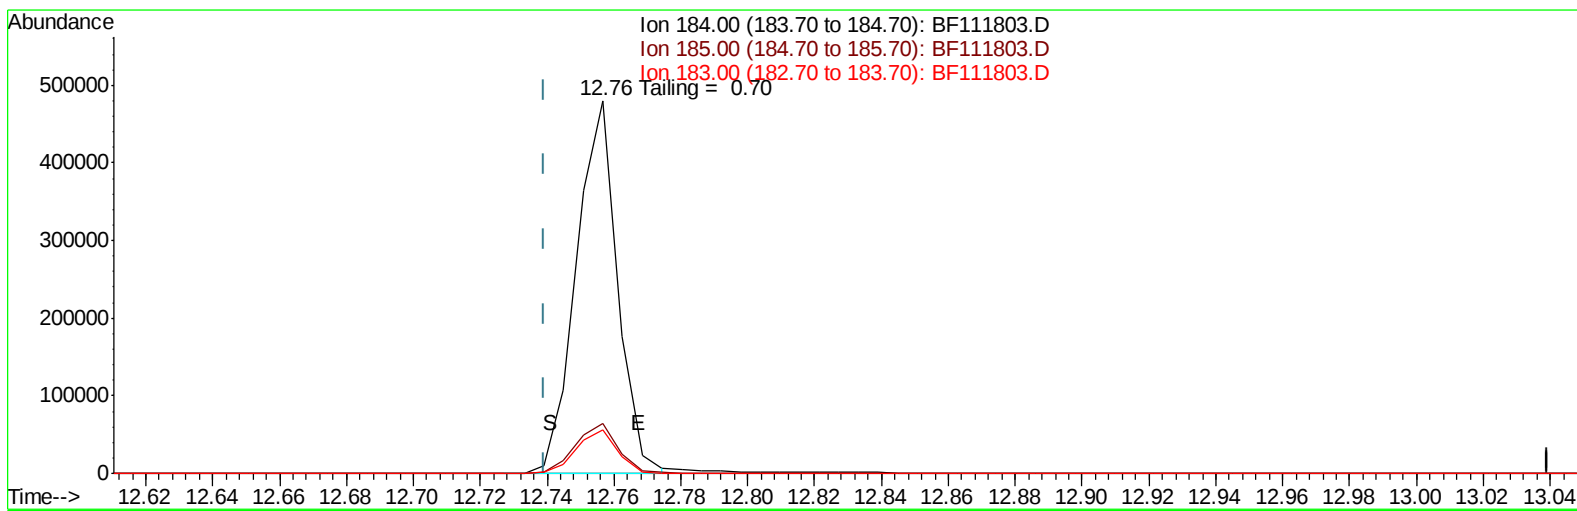

TIC: BF111803.D

(77) Benzidine

12.757min (+0.017) 0.00ng

response 421064

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	13.28
183.00	11.60	11.52
0.00	0.00	0.00