

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF010219\
 Data File : BF111807.D
 Acq On : 2 Jan 2019 13:21
 Operator : JU/SJ
 Sample : PB116085BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB116085BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.116	511	515	520	rBV	18386	19871	1.14%	0.155%
2	5.534	582	586	595	rBV	614610	522090	30.08%	4.067%
3	6.534	753	756	767	rBV	578985	554813	31.96%	4.322%
4	6.675	776	780	784	rBV	690295	575552	33.16%	4.484%
5	6.904	815	819	822	rBV	1186118	1044335	60.16%	8.136%
6	7.057	841	845	849	rBV	545061	457252	26.34%	3.562%
7	7.457	908	913	916	rBV	357148	342415	19.73%	2.668%
8	8.186	1032	1037	1040	rBV	1533241	1367072	78.75%	10.650%
9	9.257	1214	1219	1222	rBV	814862	718265	41.38%	5.596%
10	9.939	1330	1335	1344	rBV	1894016	1648911	94.99%	12.846%
11	10.727	1465	1469	1478	rBV	318563	289199	16.66%	2.253%
12	11.427	1584	1588	1591	rBV	2032309	1735909	100.00%	13.524%
13	13.004	1852	1856	1860	rVB	1026945	813455	46.86%	6.337%
14	14.062	2032	2036	2040	rVB	1641156	1482532	85.40%	11.550%
15	14.527	2111	2115	2117	rBV	31951	30577	1.76%	0.238%
16	14.839	2165	2168	2174	rVB	37934	41237	2.38%	0.321%
17	15.186	2223	2227	2233	rVB2	41314	54404	3.13%	0.424%
18	15.551	2284	2289	2298	rVB	749179	1013080	58.36%	7.892%
19	16.021	2365	2369	2373	rVB2	39571	55538	3.20%	0.433%
20	16.539	2454	2457	2465	rVB3	41161	69650	4.01%	0.543%


Sum of corrected areas: 12836157

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF010219\
Data File : BF111807.D
Acq On : 2 Jan 2019 13:21
Operator : JU/SJ
Sample : PB116085BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB116085BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF121918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

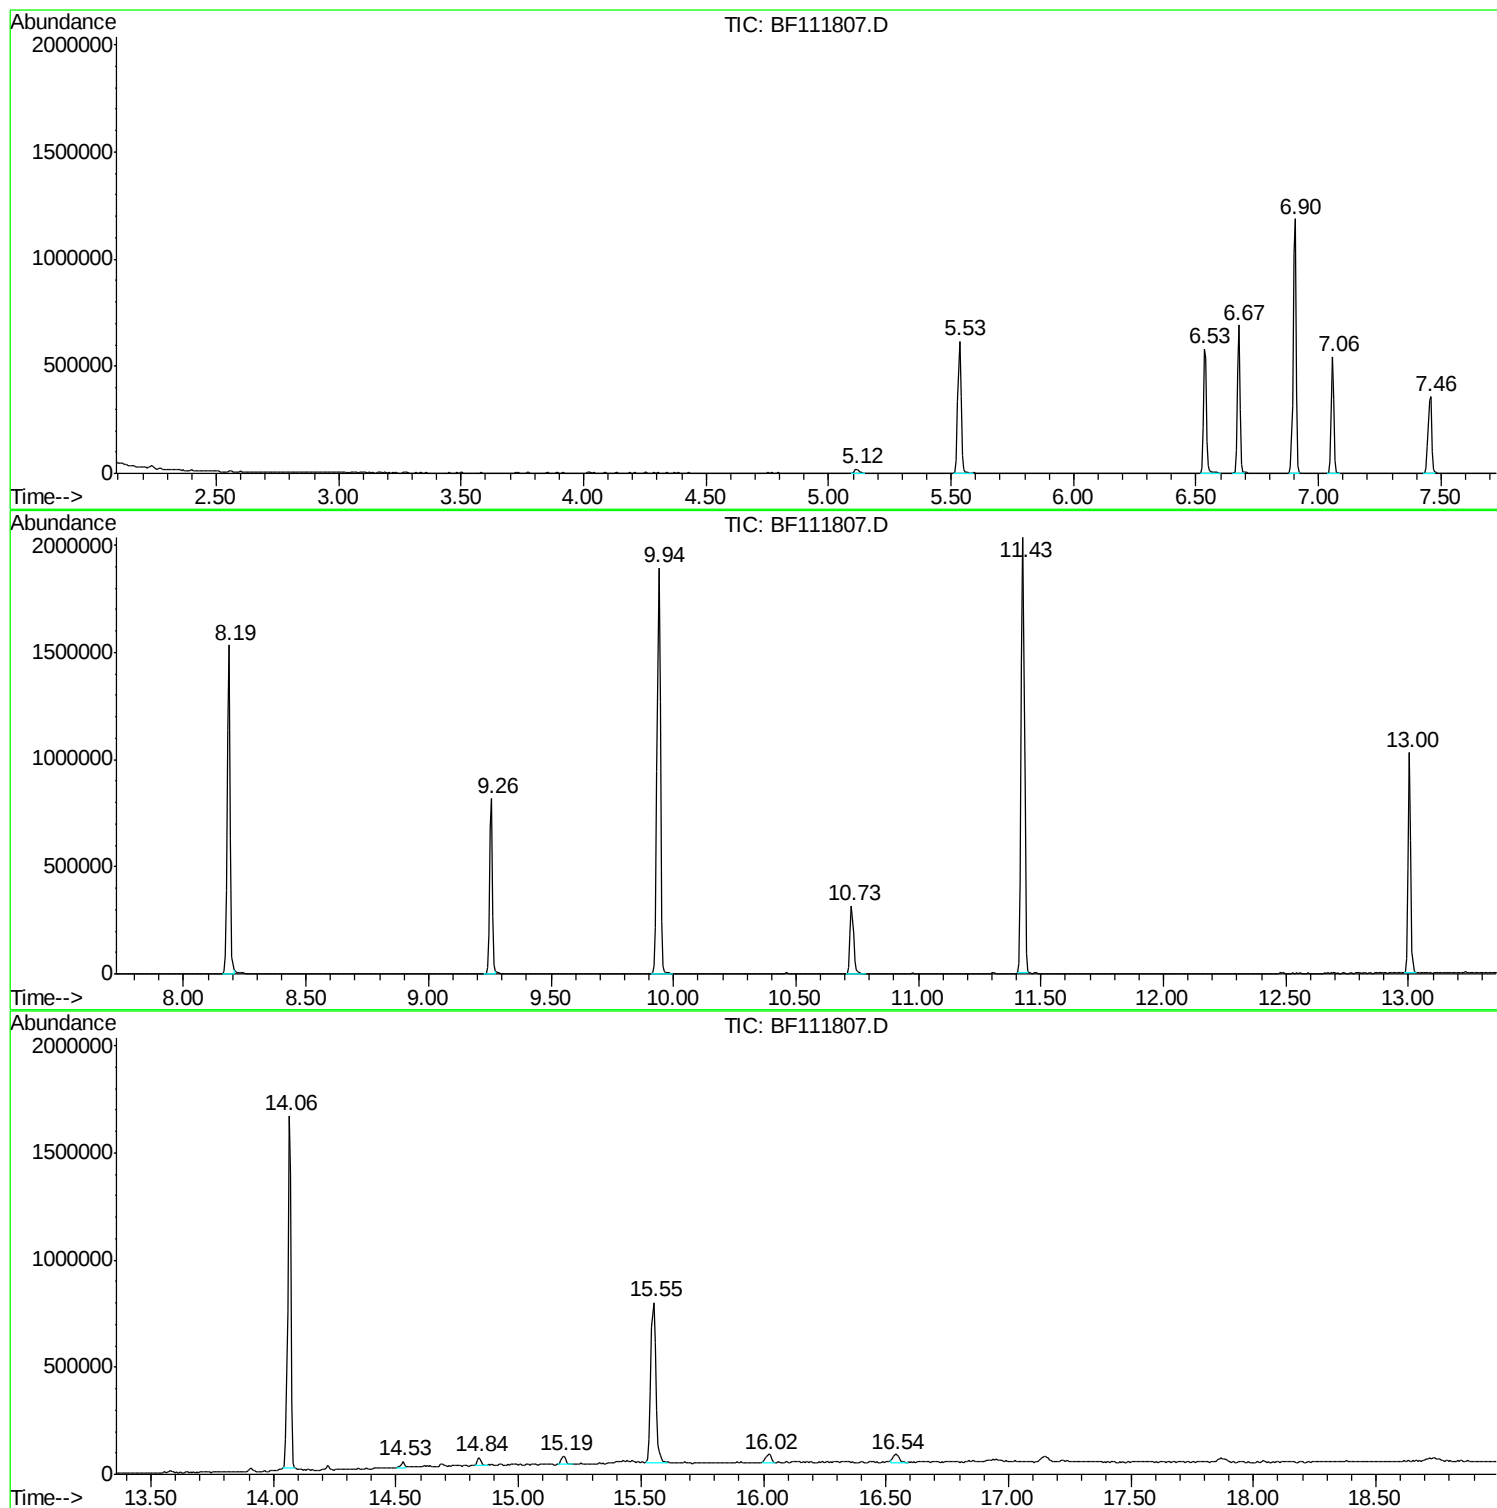

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF010219\
Data File : BF111807.D
Acq On : 2 Jan 2019 13:21
Operator : JU/SJ
Sample : PB116085BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB116085BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF121918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.67 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.67	11.02 ng	575552	1,4-Dichlorobenzene-d4	6.90

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	12
4		1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	9
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

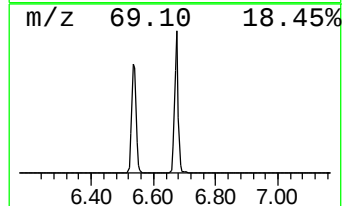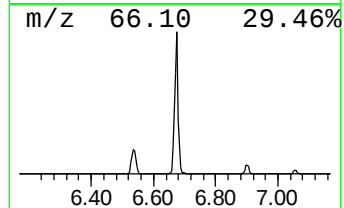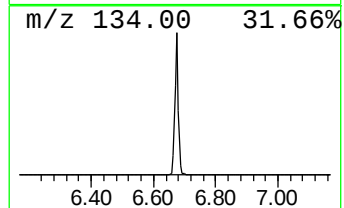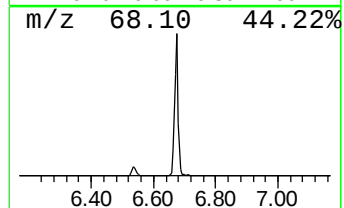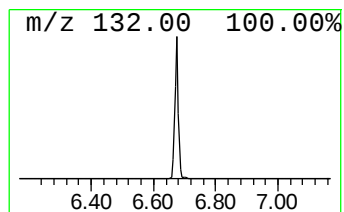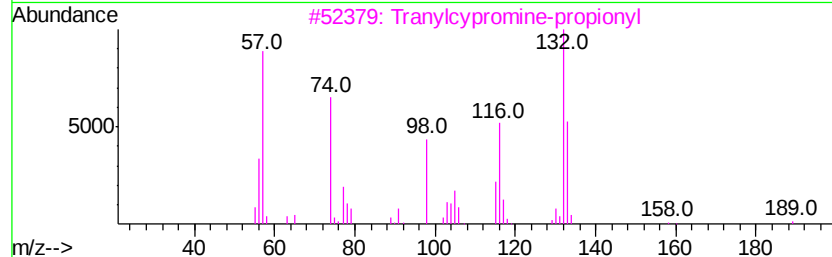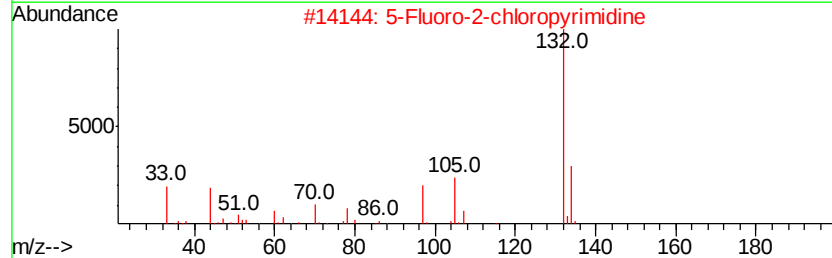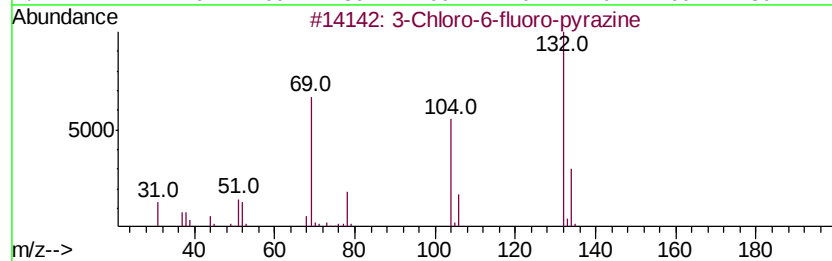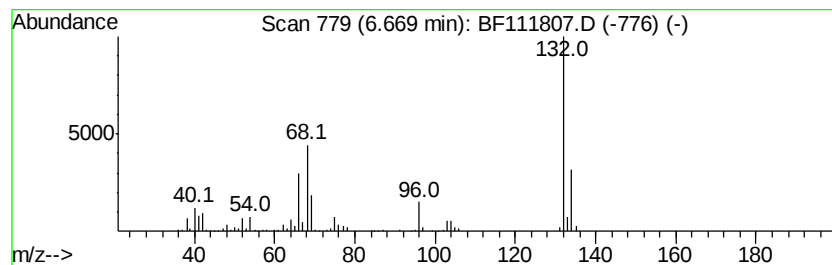

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF010219\
Data File : BF111807.D
Acq On : 2 Jan 2019 13:21
Operator : JU/SJ
Sample : PB116085BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB116085BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.67	6.67	11.0	ng	575552	1	6.90	1044340	20.0