


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010319\
 Data File : BF111816.D
 Acq On : 3 Jan 2019 12:31
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 19 17:39:39 2018

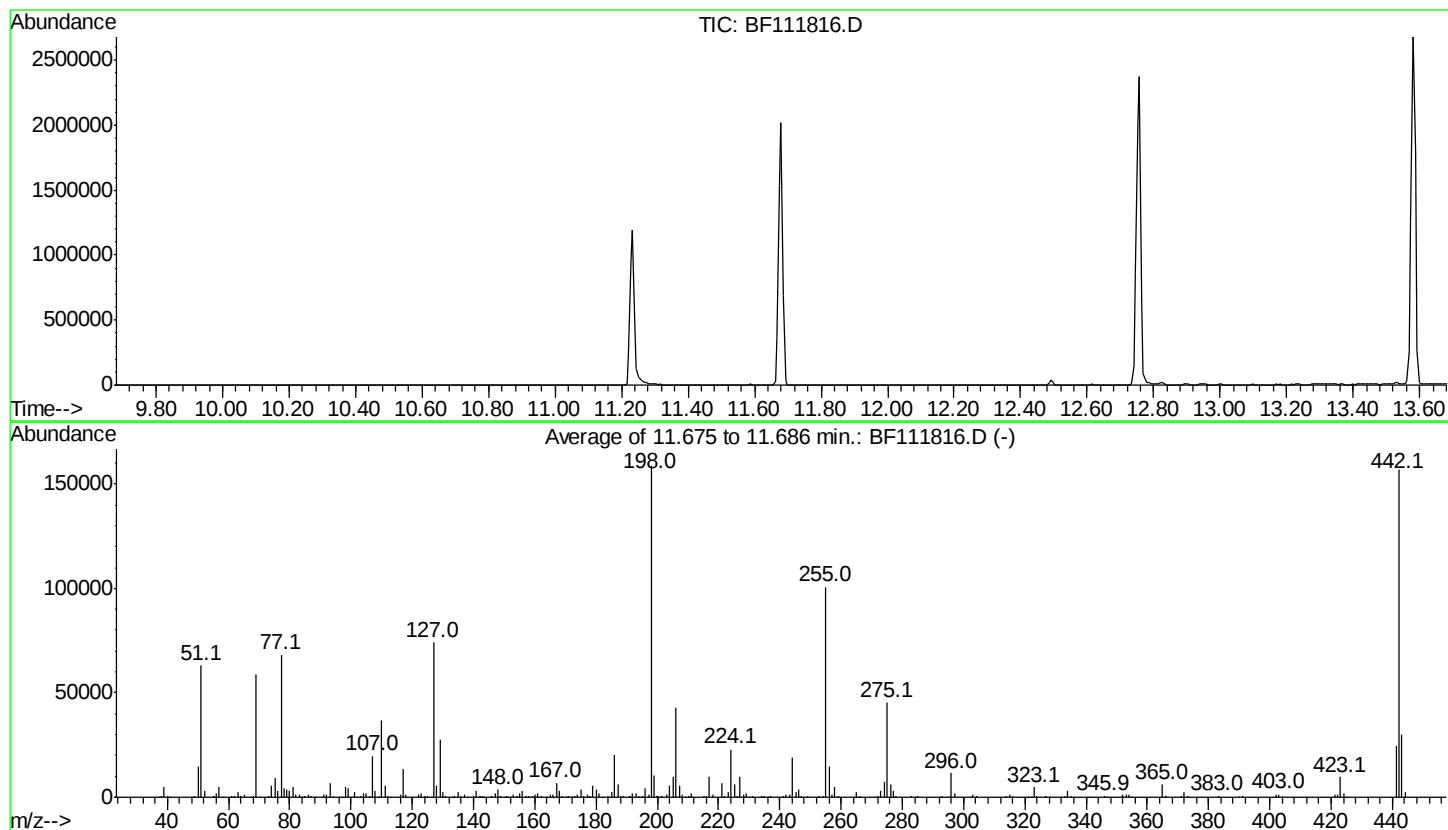

AutoFind: Scans 1630, 1631, 1632; Background Corrected with Scan 1625

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.7	63066	PASS
68	69	0.00	2	1.4	843	PASS
69	198	0.00	100	36.9	58598	PASS
70	69	0.00	2	0.5	284	PASS
127	198	10	80	46.7	74125	PASS
197	198	0.00	2	0.7	1078	PASS
198	198	100	100	100.0	158749	PASS
199	198	5	9	6.6	10536	PASS
275	198	10	60	28.5	45256	PASS
365	198	1	100	3.8	6021	PASS
441	198	0.01	100	15.4	24491	PASS
442	198	50	100	98.7	156632	PASS
443	442	15	24	19.1	29917	PASS