

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010322\
 Data File : BF126449.D
 Acq On : 3 Jan 2022 11:29
 Operator : JU/CG
 Sample : M5244-06 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CONC-2A

Quant Time: Jan 03 12:00:26 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 30 04:30:49 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.798	152	133024	20.000	ng	0.00
21) Naphthalene-d8	8.080	136	496053	20.000	ng	0.00
39) Acenaphthene-d10	9.833	164	200228	20.000	ng	0.00
64) Phenanthrene-d10	11.316	188	310053	20.000	ng	0.00
76) Chrysene-d12	13.957	240	240614	20.000	ng	0.00
86) Perylene-d12	15.398	264	270251	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.404	112	177728	19.187	ng	0.00
7) Phenol-d6	6.422	99	206386	17.202	ng	0.00
23) Nitrobenzene-d5	7.351	82	124630	12.900	ng	-0.01
42) 2,4,6-Tribromophenol	10.616	330	24982	16.146	ng	0.00
45) 2-Fluorobiphenyl	9.151	172	180074	15.826	ng	0.00
79) Terphenyl-d14	12.898	244	174195	14.066	ng	0.00
Target Compounds						
60) Diethylphthalate	10.245	149	26339	2.186	ng	Qvalue 99
80) Butylbenzylphthalate	13.392	149	1090392	121.015	ng	# 94
84) Bis(2-ethylhexyl)phtha...	13.945	149	1158641	124.079	ng	99
85) Di-n-octyl phthalate	14.533	149	89831	5.547	ng	# 37


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010322\
Data File : BF126449.D
Acq On : 3 Jan 2022 11:29
Operator : JU/CG
Sample : M5244-06 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CONC-2A

Quant Time: Jan 03 12:00:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 30 04:30:49 2021
Response via : Initial Calibration




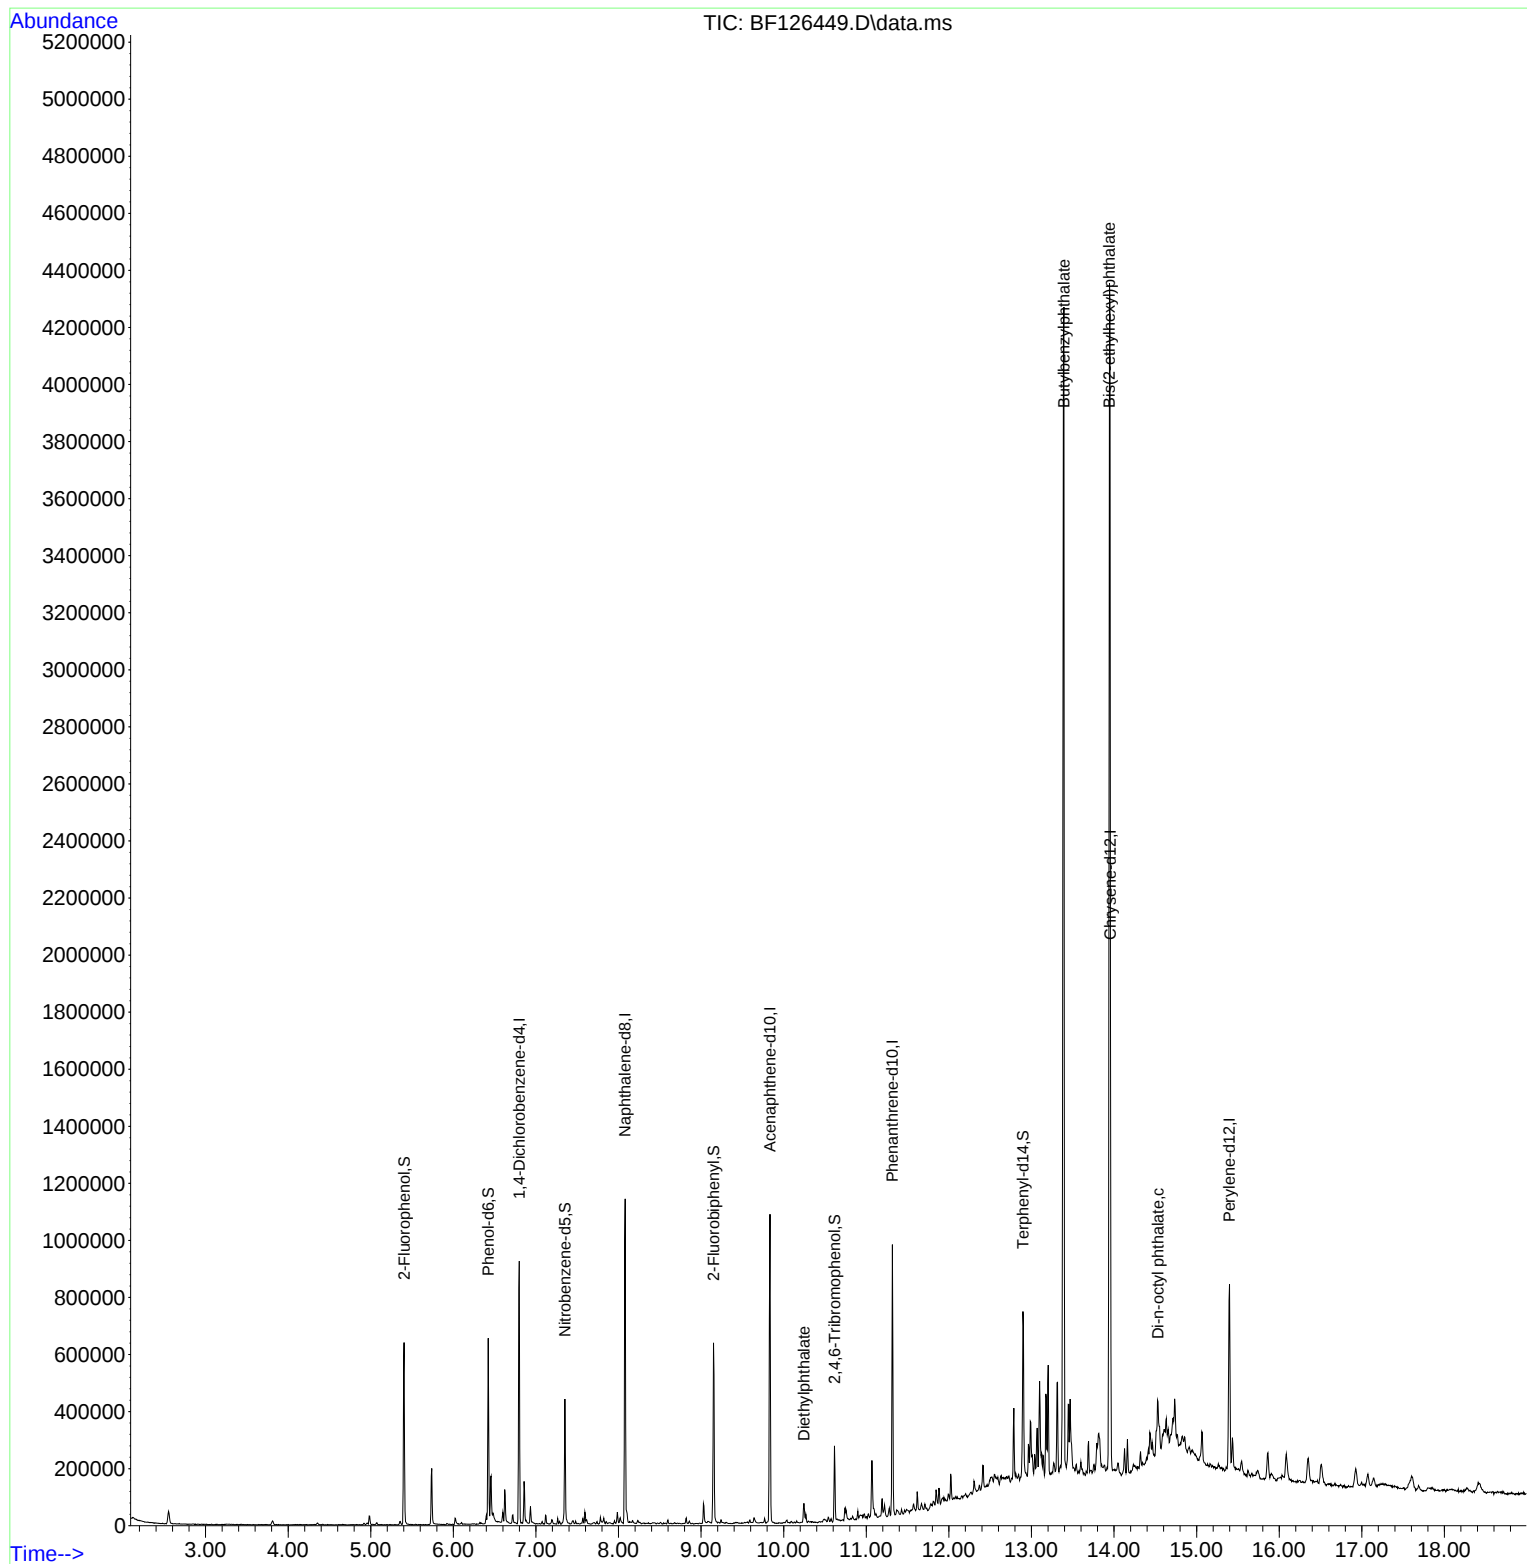


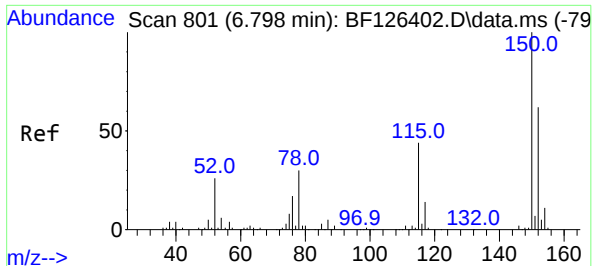

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.798 min Scan# 801
Delta R.T. 0.000 min
Lab File: BF126449.D
Acq: 3 Jan 2022 11:29




Instrument :
BNA_F
ClientSampleId :
CONC-2A

Tgt Ion:152 Resp: 133024
Ion Ratio Lower Upper
152 100
150 155.6 128.1 192.1
115 64.0 56.7 85.1

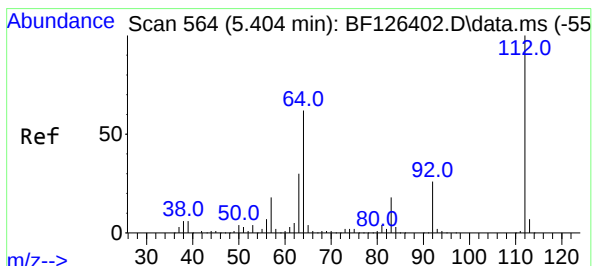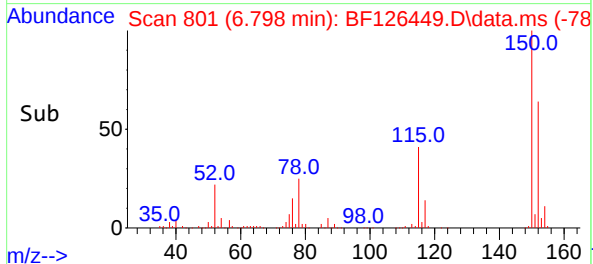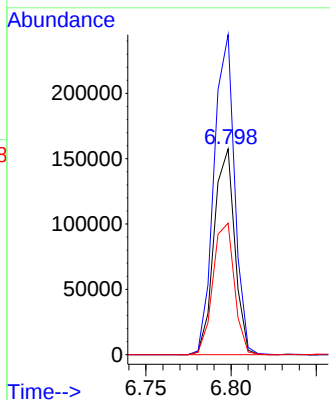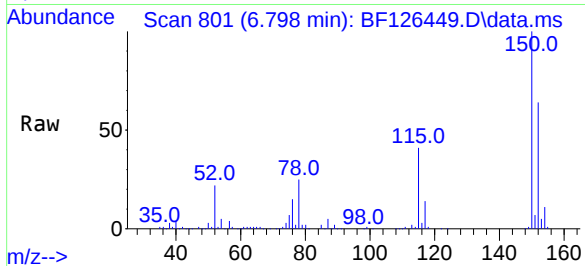


#5
2-Fluorophenol
Concen: 19.187 ng
RT: 5.404 min Scan# 564
Delta R.T. 0.000 min
Lab File: BF126449.D
Acq: 3 Jan 2022 11:29


Tgt Ion:112 Resp: 177728
Ion Ratio Lower Upper
112 100
64 56.1 49.5 74.3
63 26.1 23.9 35.9

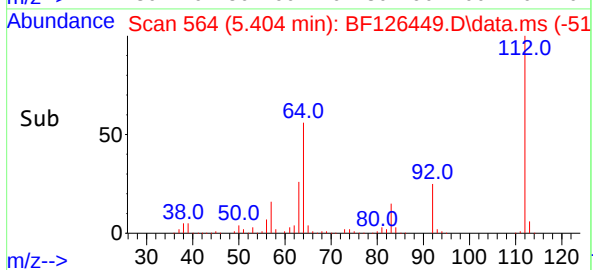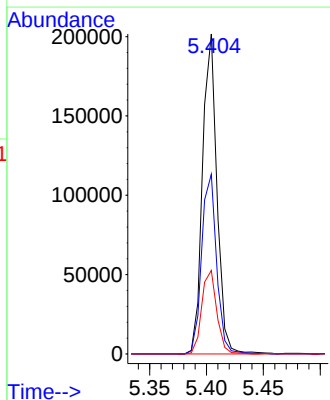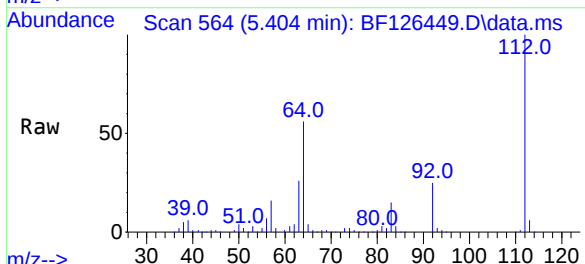


Abundance Scan 738 (6.428 min): BF126402.D\data.ms (-73

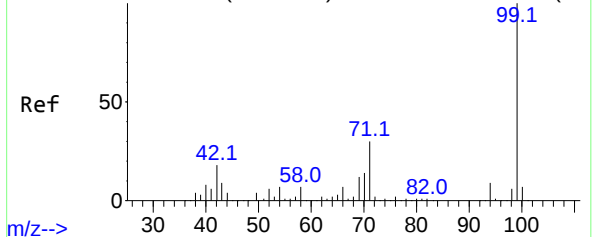


m/z--> Scan 737 (6.422 min): BF126449.D\data.ms

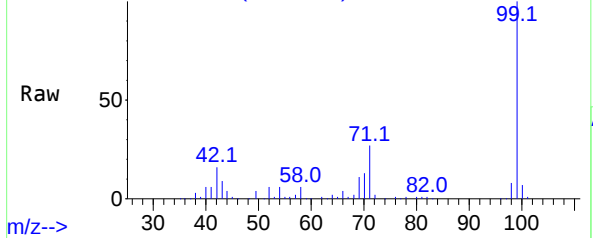


m/z--> Abundance Scan 737 (6.422 min): BF126449.D\data.ms (-68

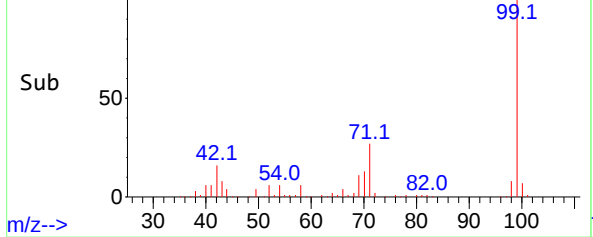


m/z--> Abundance Scan 1019 (8.080 min): BF126402.D\data.ms (-1

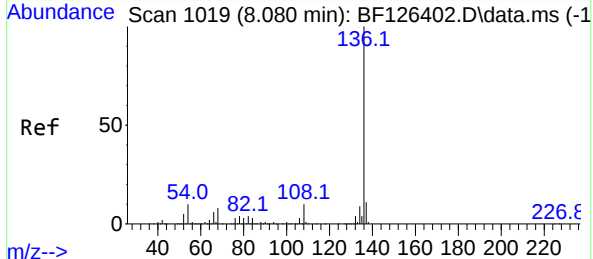

m/z--> Abundance Scan 1019 (8.080 min): BF126449.D\data.ms

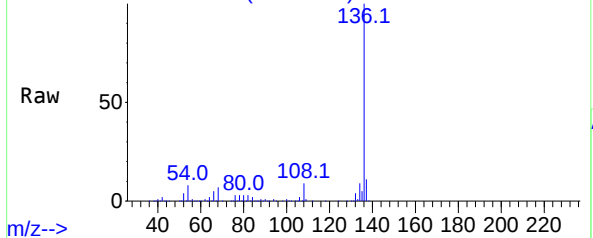

m/z--> Abundance Scan 1019 (8.080 min): BF126449.D\data.ms (-9

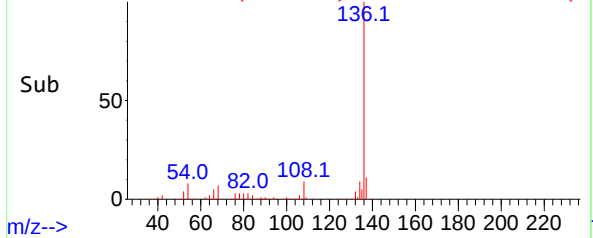

m/z--> Abundance Scan 1019 (8.080 min): BF126449.D\data.ms (-9



m/z--> Abundance Scan 1019 (8.080 min): BF126449.D\data.ms (-9

m/z--> Abundance Scan 1019 (8.080 min): BF126449.D\data.ms (-9

m/z--> Abundance Scan 1019 (8.080 min): BF126449.D\data.ms (-9

m/z--> Abundance Scan 1019 (8.080 min): BF126449.D\data.ms (-9

m/z--> Abundance Scan 1019 (8.080 min): BF126449.D\data.ms (-9

m/z--> Abundance Scan 1019 (8.080 min): BF126449.D\data.ms (-9


m/z--> Abundance Scan 1019 (8.080 min): BF126449.D\data.ms (-9

#7
Phenol-d6
Concen: 17.202 ng
RT: 6.422 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF126449.D
Acq: 3 Jan 2022 11:29

Instrument :
BNA_F
ClientSampleId :
CONC-2A

Tgt Ion: 99 Resp: 206386


Ion	Ratio	Lower	Upper
99	100		
42	15.7	14.2	21.4
71	26.7	24.3	36.5

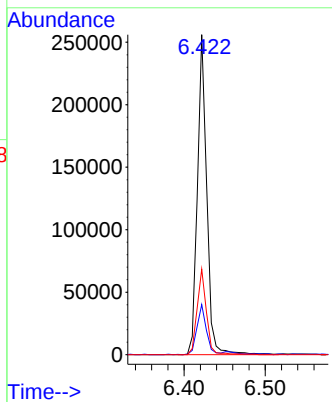


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.080 min Scan# 1019
Delta R.T. 0.000 min
Lab File: BF126449.D
Acq: 3 Jan 2022 11:29

Tgt Ion: 136 Resp: 496053

Ion	Ratio	Lower	Upper
136	100		
137	10.7	8.6	13.0
54	8.1	7.8	11.6
68	6.9	6.3	9.5

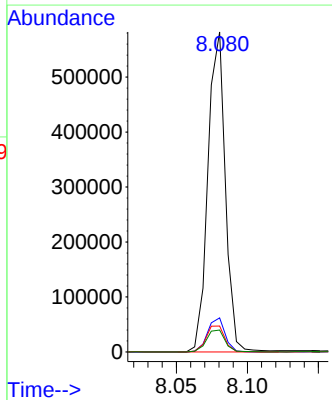

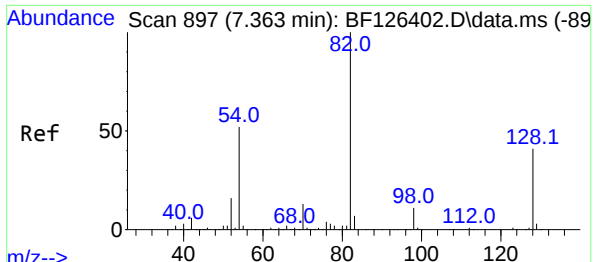

#23

Nitrobenzene-d5

Concen: 12.900 ng

RT: 7.351 min Scan# 89

Delta R.T. -0.012 min

Lab File: BF126449.D

Acq: 3 Jan 2022 11:29

Instrument :

BNA_F

ClientSampleId :

CONC-2A





Tgt Ion: 82 Resp: 124630

Ion Ratio Lower Upper

82 100

128 43.0 32.7 49.1

54 50.2 41.7 62.5

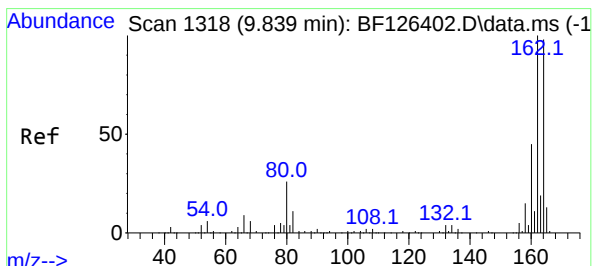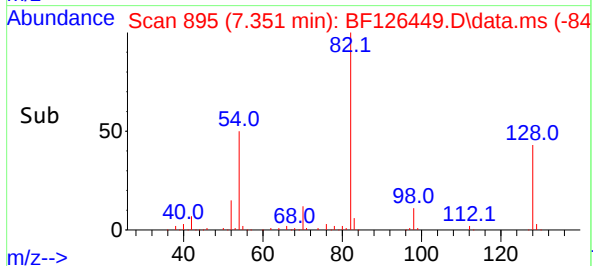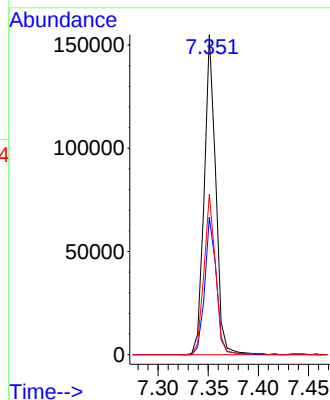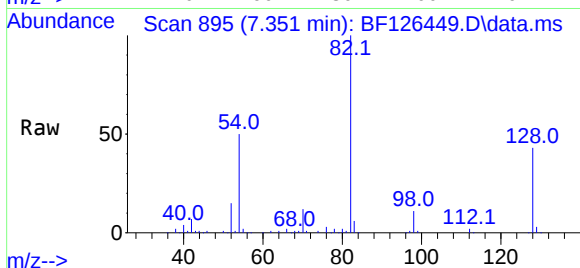

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.833 min Scan# 1317

Delta R.T. -0.006 min

Lab File: BF126449.D

Acq: 3 Jan 2022 11:29




Tgt Ion:164 Resp: 200228


Ion Ratio Lower Upper

164 100

162 99.9 81.4 122.0


160 44.2 36.6 54.8

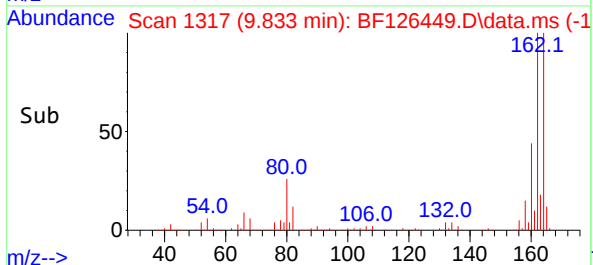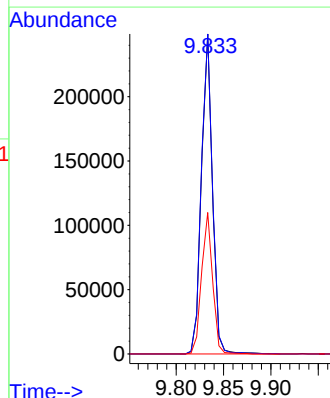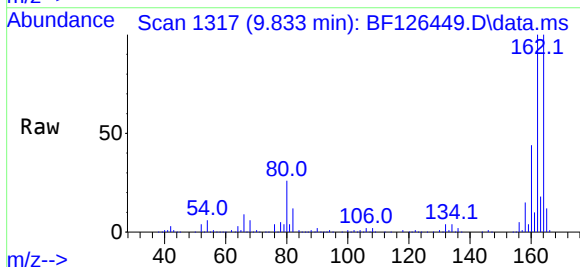



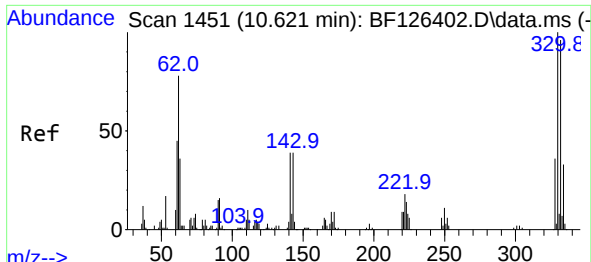


#42
2,4,6-Tribromophenol
Concen: 16.146 ng
RT: 10.616 min Scan# 1450
Delta R.T. -0.006 min
Lab File: BF126449.D
Acq: 3 Jan 2022 11:29


Instrument :
BNA_F
ClientSampleId :
CONC-2A

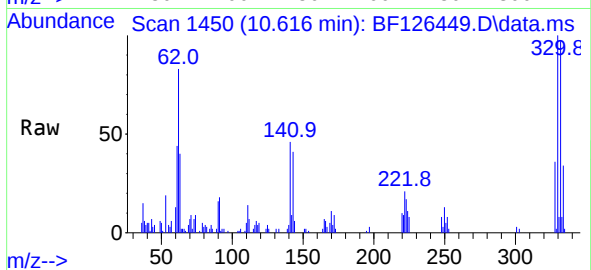



Tgt Ion:330 Resp: 24982
Ion Ratio Lower Upper
330 100
332 95.1 76.0 114.0
141 40.2 30.1 45.1

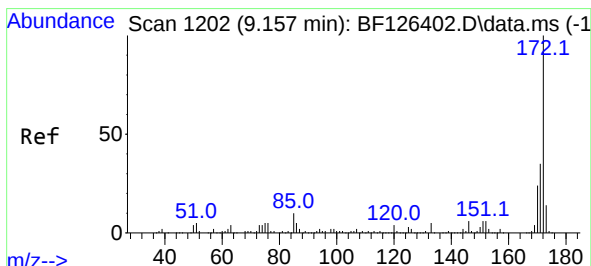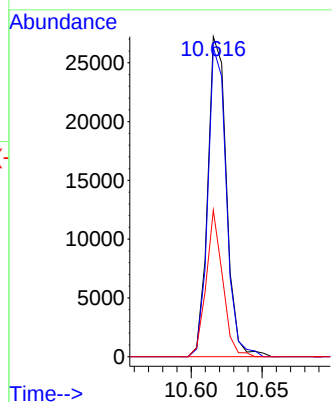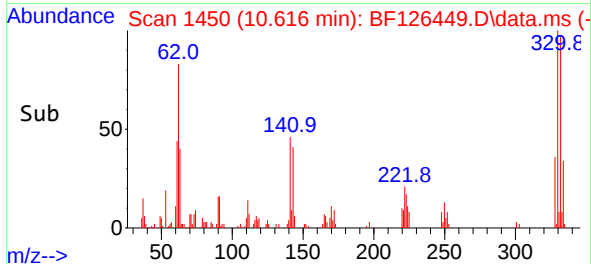


#45
2-Fluorobiphenyl
Concen: 15.826 ng
RT: 9.151 min Scan# 1201
Delta R.T. -0.006 min
Lab File: BF126449.D
Acq: 3 Jan 2022 11:29

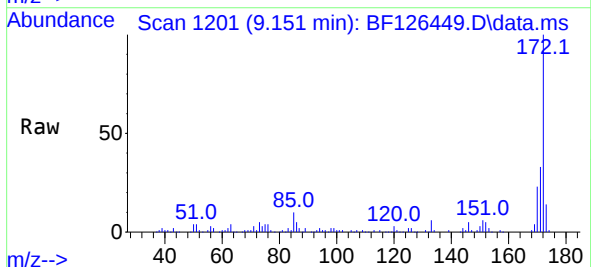

Tgt Ion:172 Resp: 180074
Ion Ratio Lower Upper
172 100
171 33.2 28.3 42.5
170 22.9 19.0 28.6



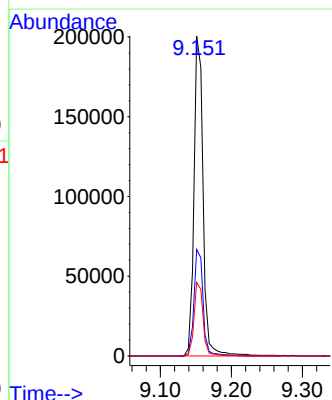
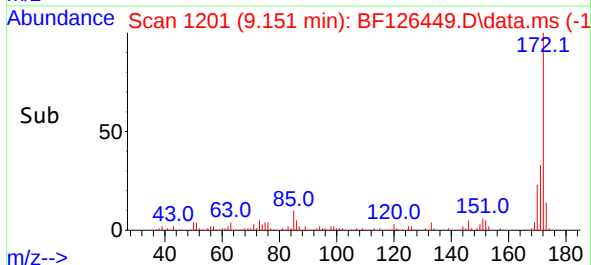


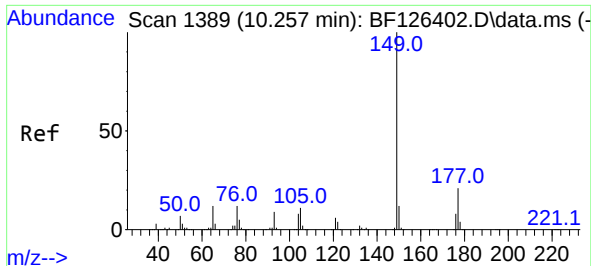

#60
Diethylphthalate
Concen: 2.186 ng
RT: 10.245 min Scan# 11
Delta R.T. -0.012 min
Lab File: BF126449.D
Acq: 3 Jan 2022 11:29




Instrument :
BNA_F
ClientSampleId :
CONC-2A


Tgt Ion:149 Resp: 26339
Ion Ratio Lower Upper
149 100
177 21.4 16.7 25.1
150 12.8 9.8 14.8

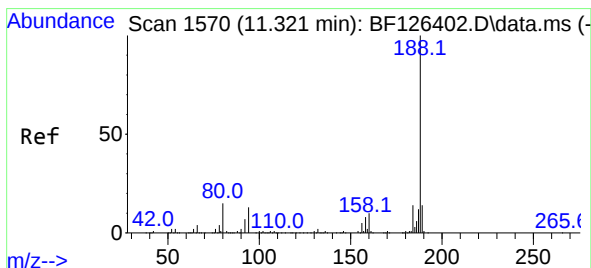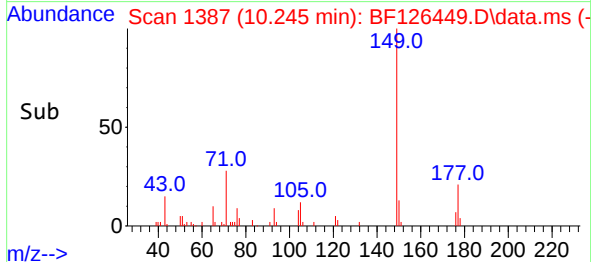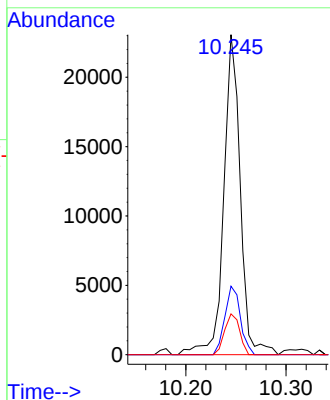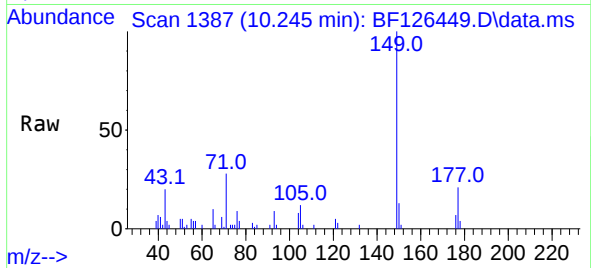

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.316 min Scan# 1569
Delta R.T. -0.006 min
Lab File: BF126449.D
Acq: 3 Jan 2022 11:29

Tgt Ion:188 Resp: 310053
Ion Ratio Lower Upper
188 100
94 14.3 10.1 15.1
80 15.2 11.8 17.6


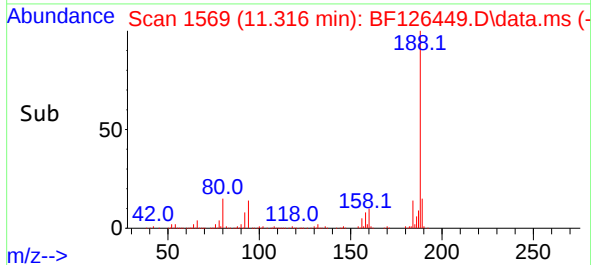
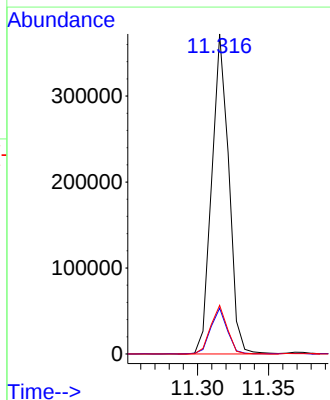
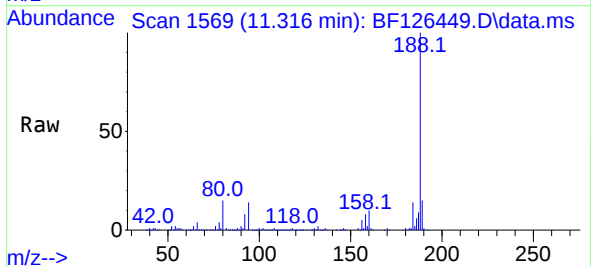


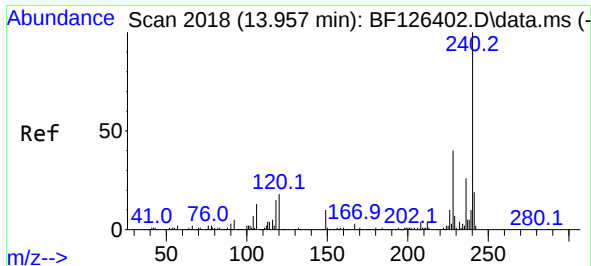

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.957 min Scan# 20
Delta R.T. -0.000 min
Lab File: BF126449.D
Acq: 3 Jan 2022 11:29




Instrument :
BNA_F
ClientSampleId :
CONC-2A


Tgt Ion:240 Resp: 240614
Ion Ratio Lower Upper
240 100
120 16.0 14.4 21.6
236 25.1 20.5 30.7

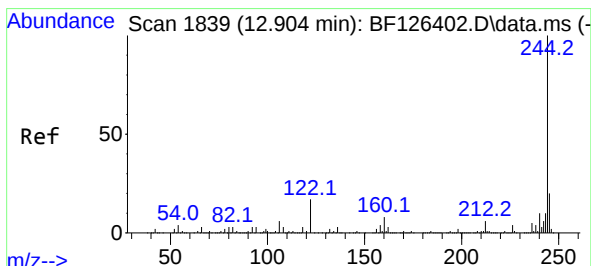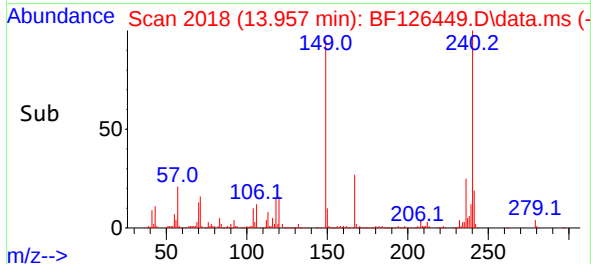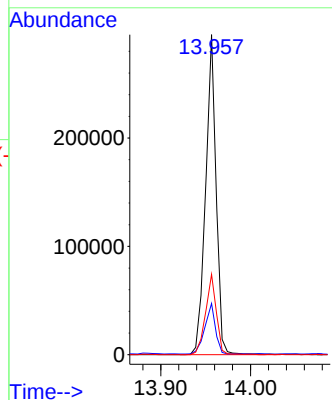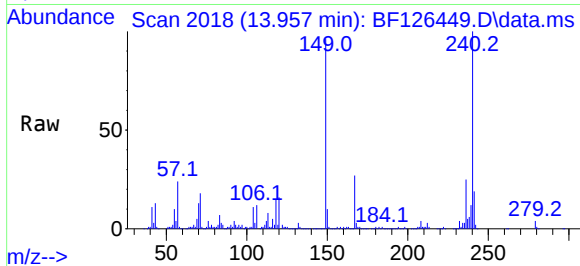

#79
Terphenyl-d14
Concen: 14.066 ng
RT: 12.898 min Scan# 1838
Delta R.T. -0.006 min
Lab File: BF126449.D
Acq: 3 Jan 2022 11:29

Tgt Ion:244 Resp: 174195
Ion Ratio Lower Upper
244 100
212 5.8 5.0 7.4
122 17.8 13.3 19.9


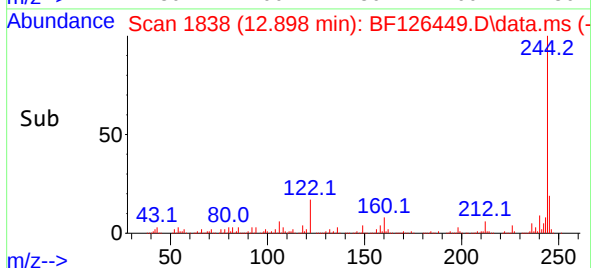
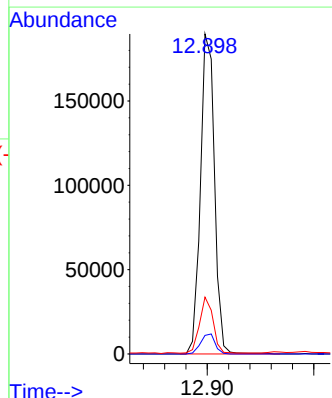
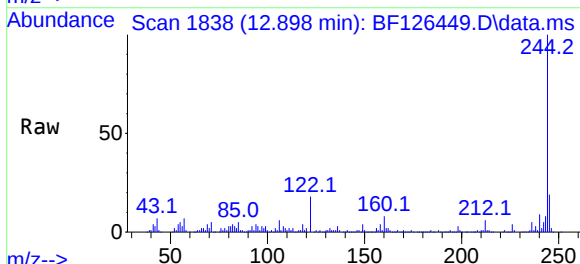


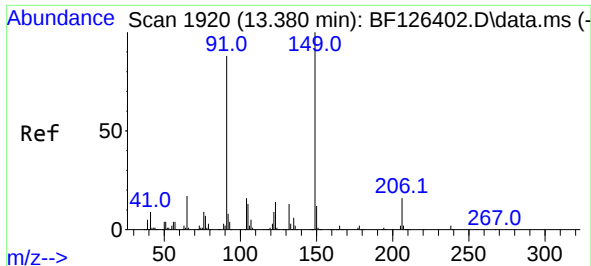

#80
Butylbenzylphthalate
Concen: 121.015 ng
RT: 13.392 min Scan# 1922
Delta R.T. 0.012 min
Lab File: BF126449.D
Acq: 3 Jan 2022 11:29




Instrument :
BNA_F
ClientSampleId :
CONC-2A


Tgt Ion:149 Resp: 1090392
Ion Ratio Lower Upper
149 100
91 82.6 70.5 105.7
206 19.0 12.6 19.0#

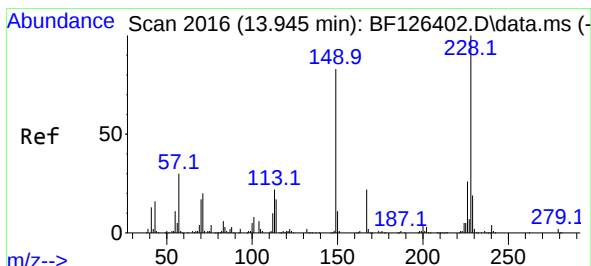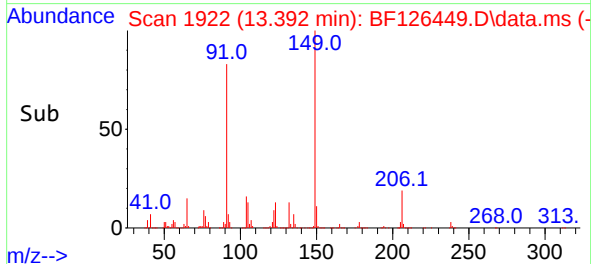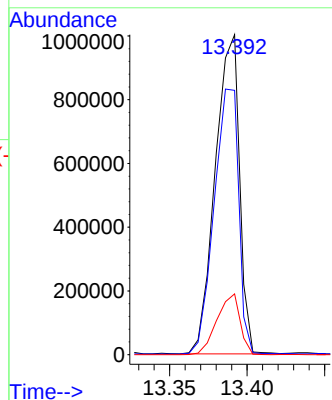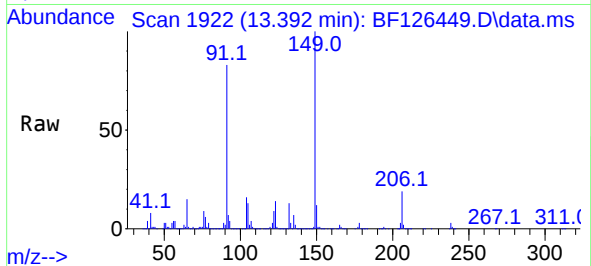

#84
Bis(2-ethylhexyl)phthalate
Concen: 124.079 ng
RT: 13.945 min Scan# 2016
Delta R.T. -0.000 min
Lab File: BF126449.D
Acq: 3 Jan 2022 11:29

Tgt Ion:149 Resp: 1158641
Ion Ratio Lower Upper
149 100
167 26.3 21.4 32.2
279 2.9 2.4 3.6


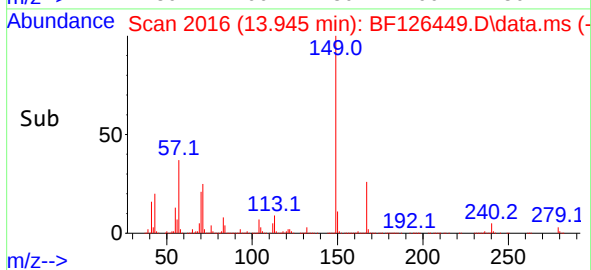
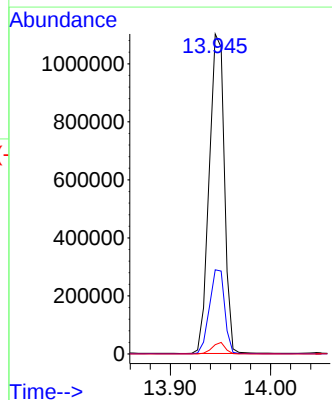
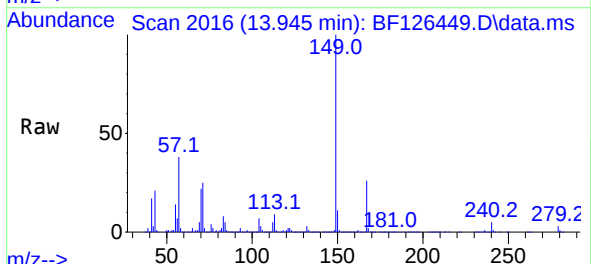


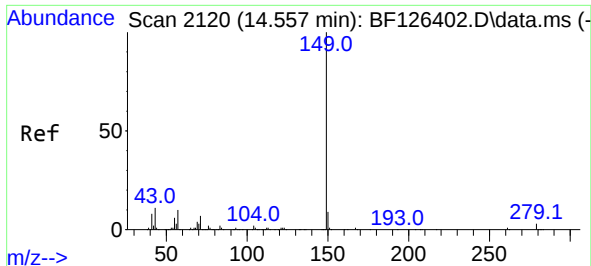

#85
Di-n-octyl phthalate
Concen: 5.547 ng
RT: 14.533 min Scan# 2116
Delta R.T. -0.024 min
Lab File: BF126449.D
Acq: 3 Jan 2022 11:29

Instrument :
BNA_F
ClientSampleId :
CONC-2A

Tgt Ion:149 Resp: 89831
Ion Ratio Lower Upper
149 100
167 8.8 1.1 1.7#
43 39.0 9.9 14.9#

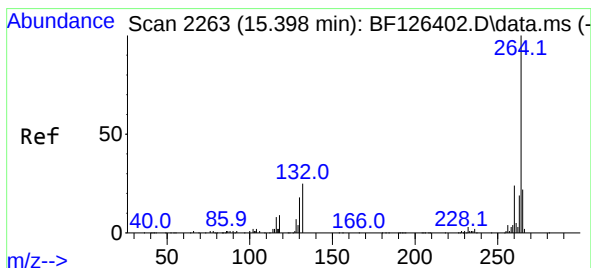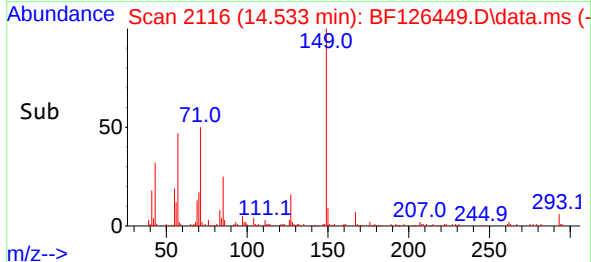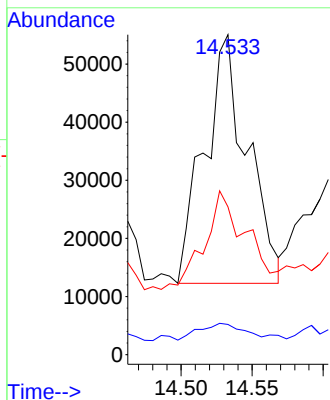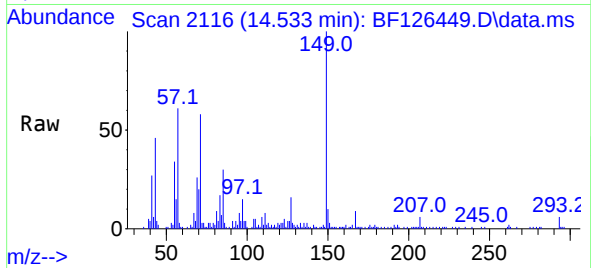

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.398 min Scan# 2263
Delta R.T. 0.000 min
Lab File: BF126449.D
Acq: 3 Jan 2022 11:29

Tgt Ion:264 Resp: 270251
Ion Ratio Lower Upper
264 100
260 24.9 19.2 28.8
265 21.5 17.4 26.2

