
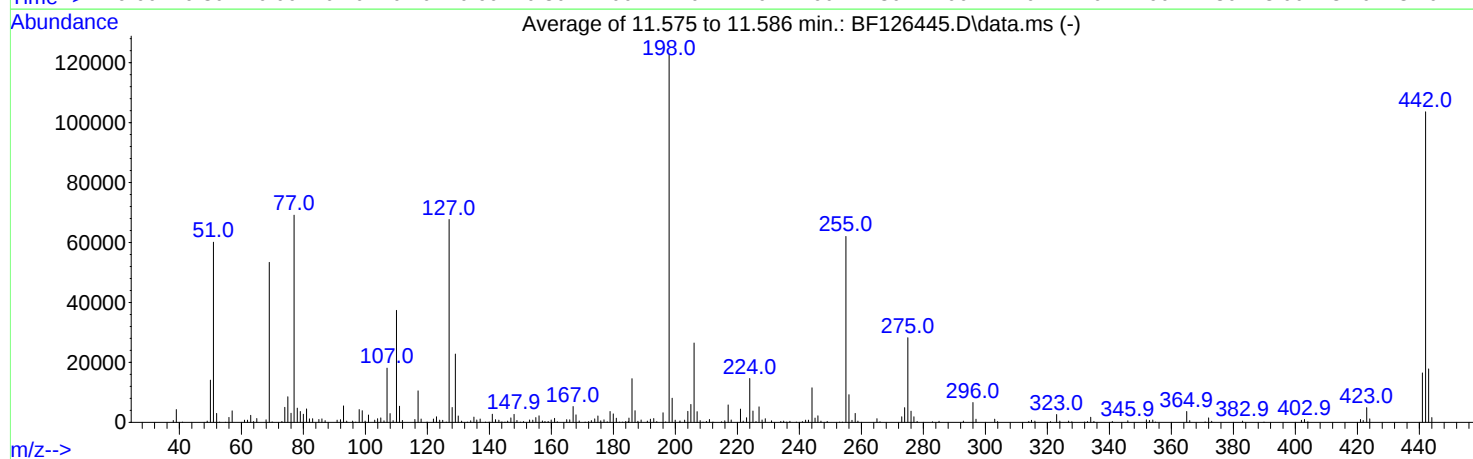


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010322\
 Data File : BF126445.D
 Acq On : 3 Jan 2022 9:05
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 30 04:30:49 2021

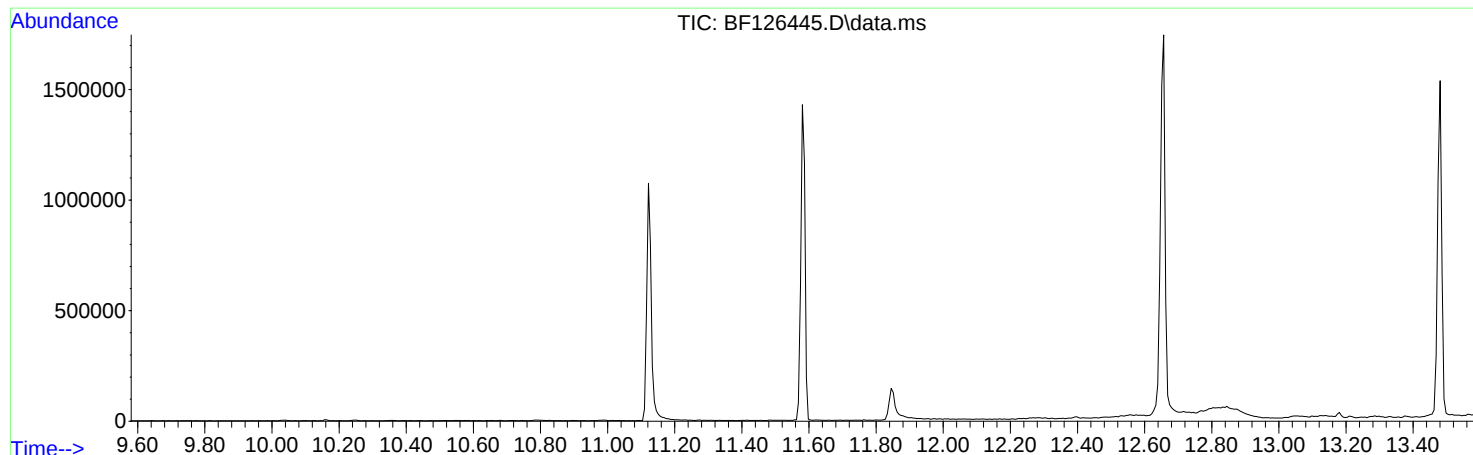




AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.0	60088	PASS
68	69	0.00	2	1.6	853	PASS
69	198	0.00	100	43.5	53365	PASS
70	69	0.00	2	0.3	151	PASS
127	198	10	80	55.2	67707	PASS
197	198	0.00	2	0.1	168	PASS
198	198	100	100	100.0	122712	PASS
199	198	5	9	6.6	8081	PASS
275	198	10	60	23.0	28230	PASS
365	198	1	100	3.0	3634	PASS
441	198	0.01	100	13.5	16511	PASS
442	442	50	100	100.0	103605	PASS
443	442	15	24	17.2	17848	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010322\
Data File : BF126445.D
Acq On : 3 Jan 2022 9:05
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 03 11:12:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 30 04:30:49 2021
Response via : Initial Calibration

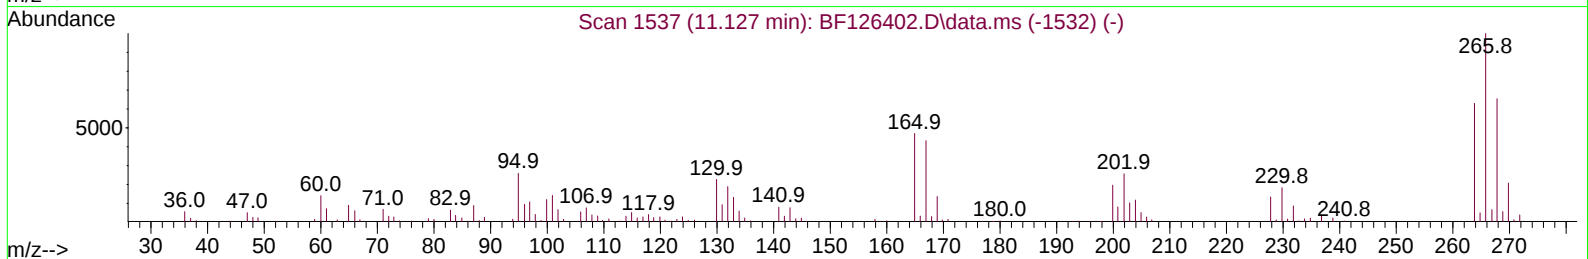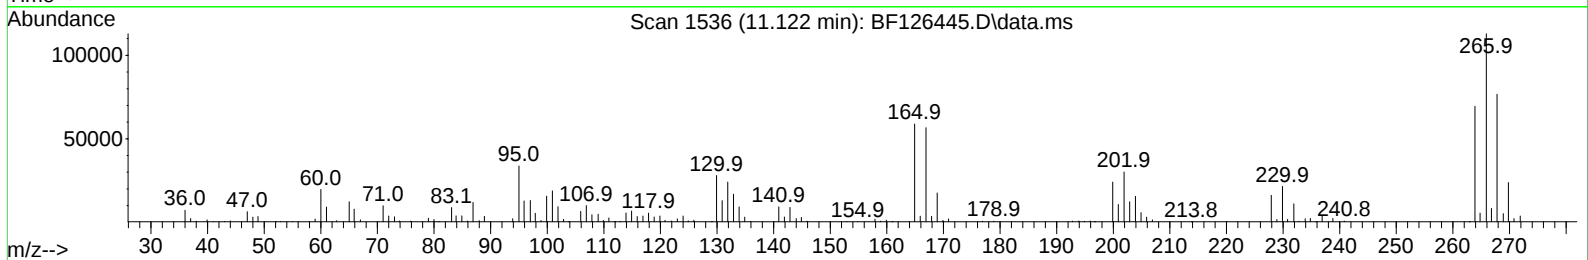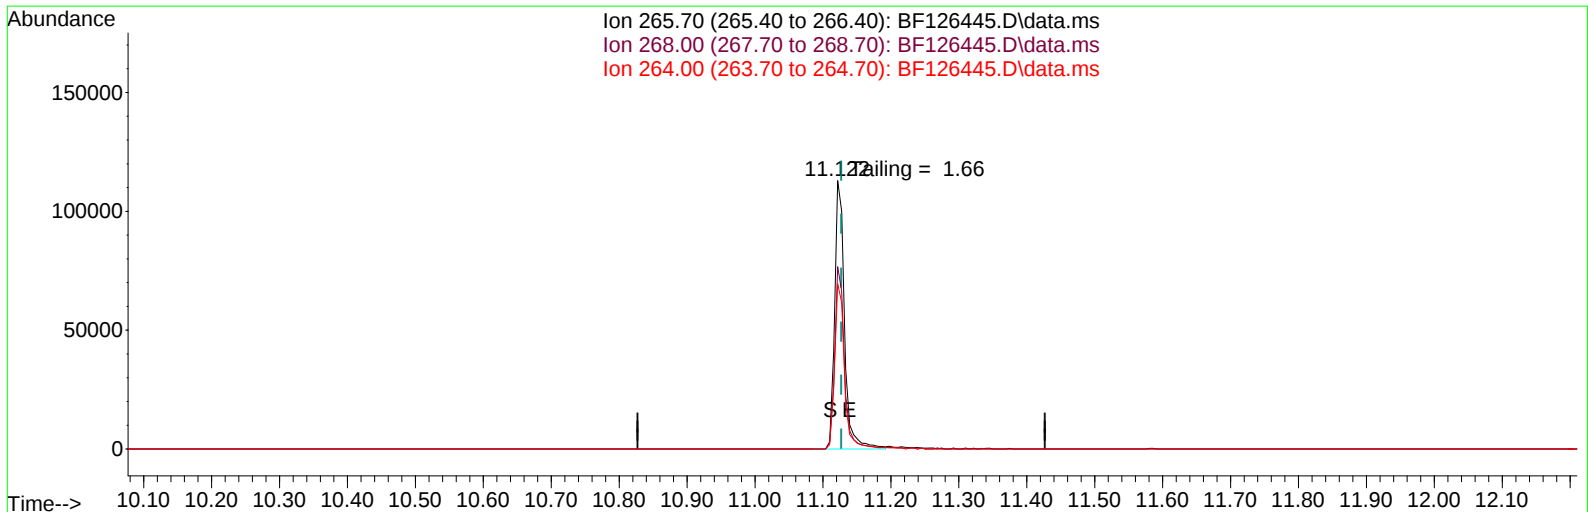

TIC: BF126445.D\data.ms

(70) Pentachlorophenol (C)

11.122min (-0.005) 58755.22 ng




response 114691

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	67.93
264.00	63.00	61.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010322\
 Data File : BF126445.D
 Acq On : 3 Jan 2022 9:05
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jan 03 11:12:12 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 30 04:30:49 2021
 Response via : Initial Calibration

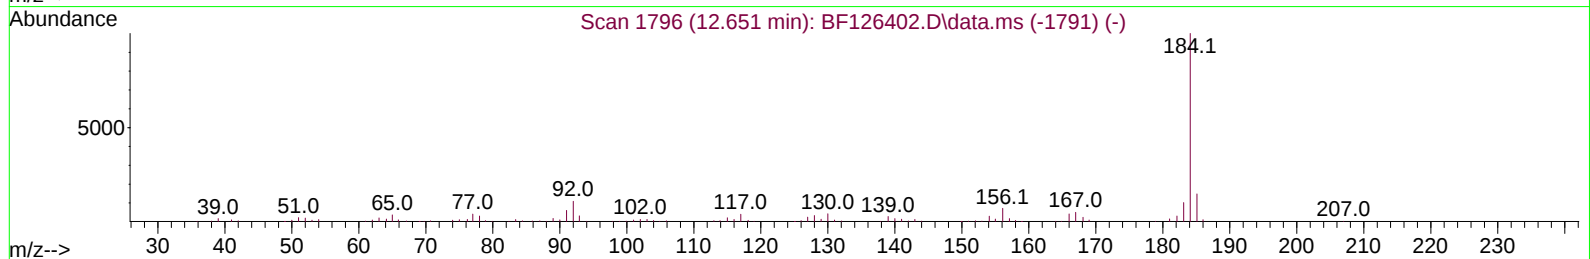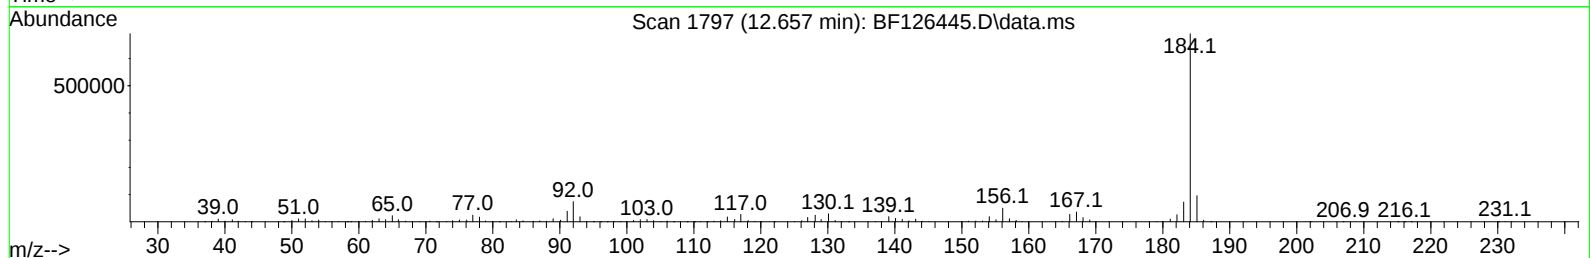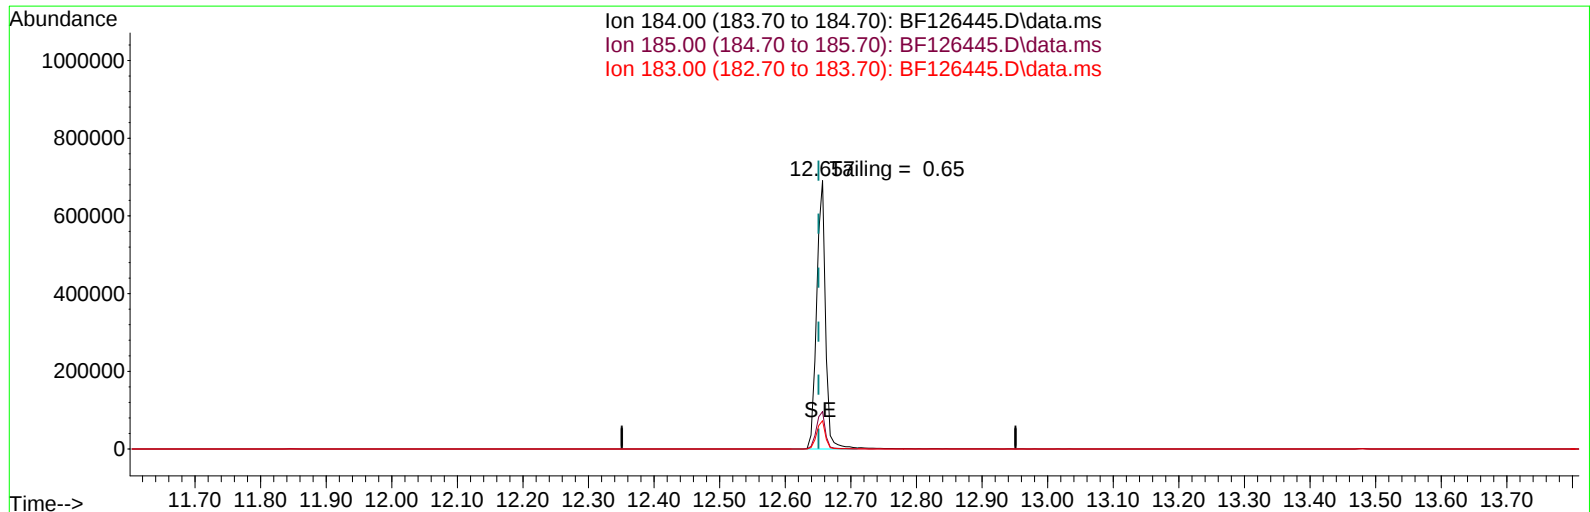

TIC: BF126445.D\data.ms

(77) Benzidine

12.657min (+ 0.006) 0.00 ng

response 656403

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	13.96
183.00	10.20	10.54
0.00	0.00	0.00

Instrument :
BNA_F
ClientSampleId :
DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/3/2022	BNA_F	<u>BF126445.D</u>
Compound Name	Response	Retention Time
DDT	239452	13.48
DDD	4290	13.18
DDE	353	12.84
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4643	244095	1.90