
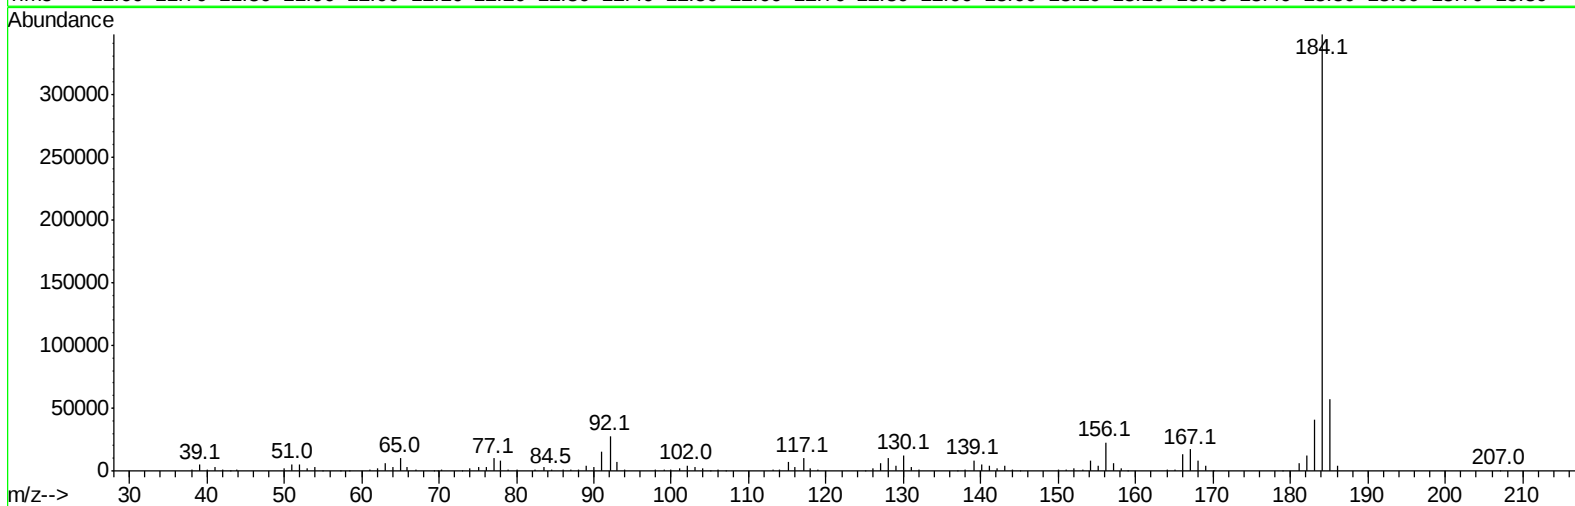


Data Path : U:\HPCHEM1\BNA F\DATA\BF010418\
Data File : BF101885.D
Acq On : 4 Jan 2018 12:26
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 05 06:54:09 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 04 14:22:17 2018
Response via : Initial Calibration

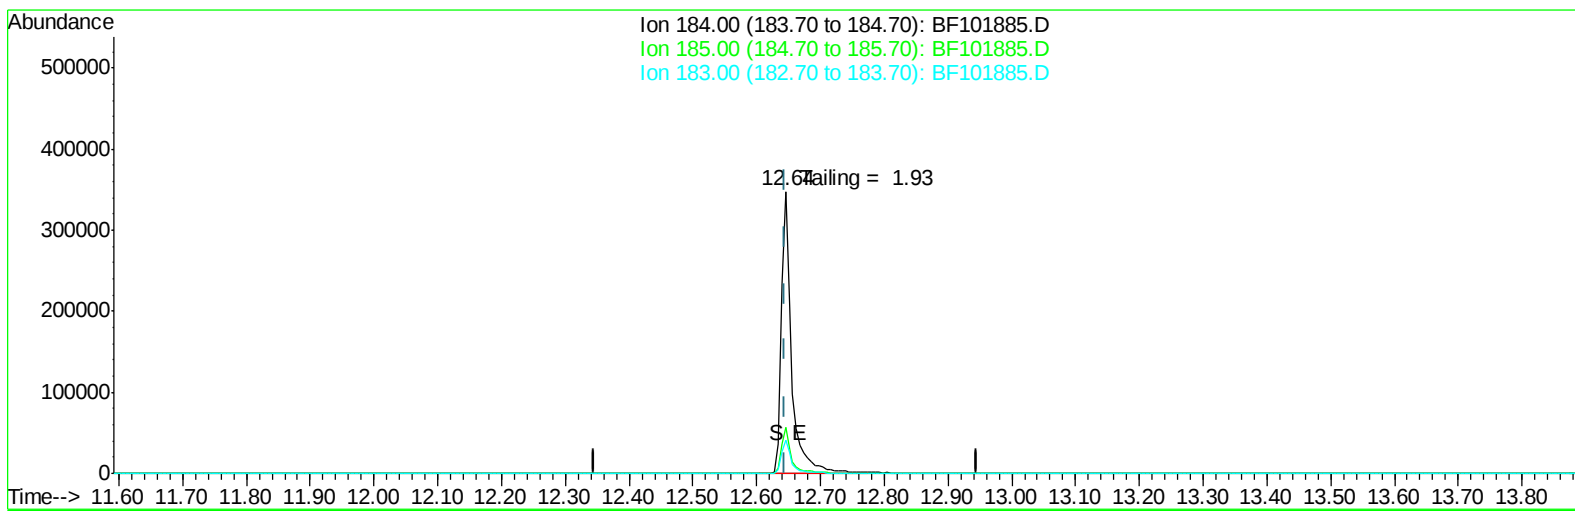

TIC: BF101885.D

(76) Benzidine


12.645min (-0.000) 17135.14ng

response 403104

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	16.38
183.00	11.60	11.73
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA F\DATA\BF010418\
Data File : BF101885.D
Acq On : 4 Jan 2018 12:26
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 05 06:54:09 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 04 14:22:17 2018
Response via : Initial Calibration

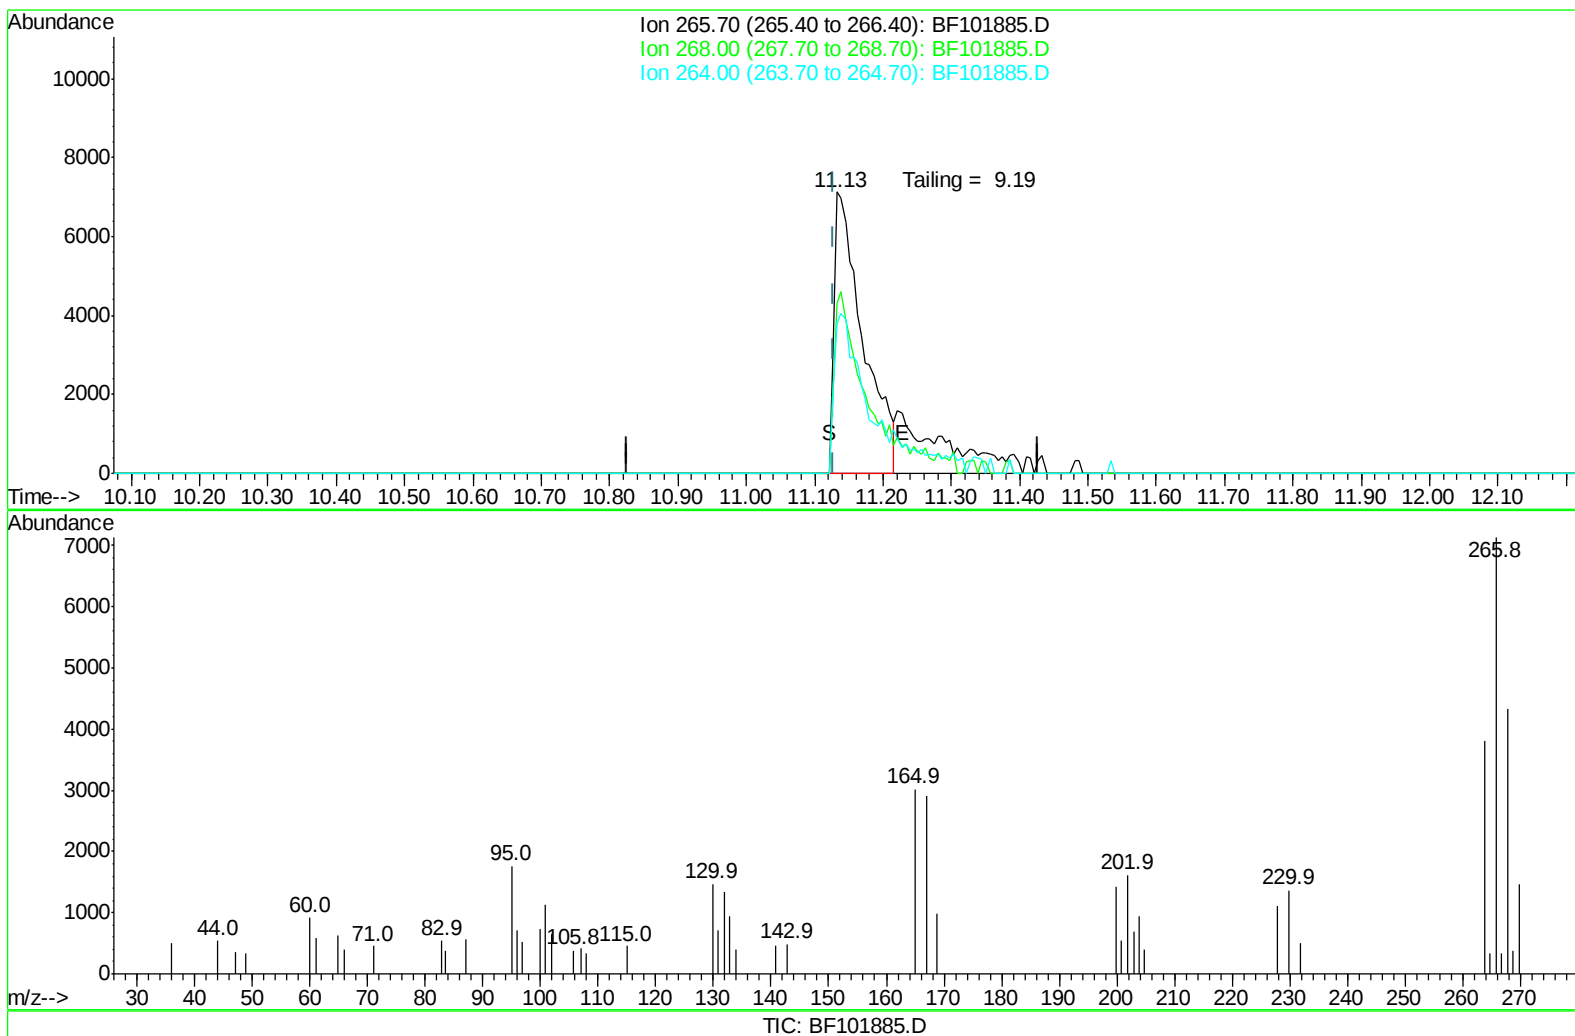

(69) Pentachlorophenol (C)

11.133min (+0.006) 0.00ng

response 20658

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.61
264.00	61.90	53.39
0.00	0.00	0.00