
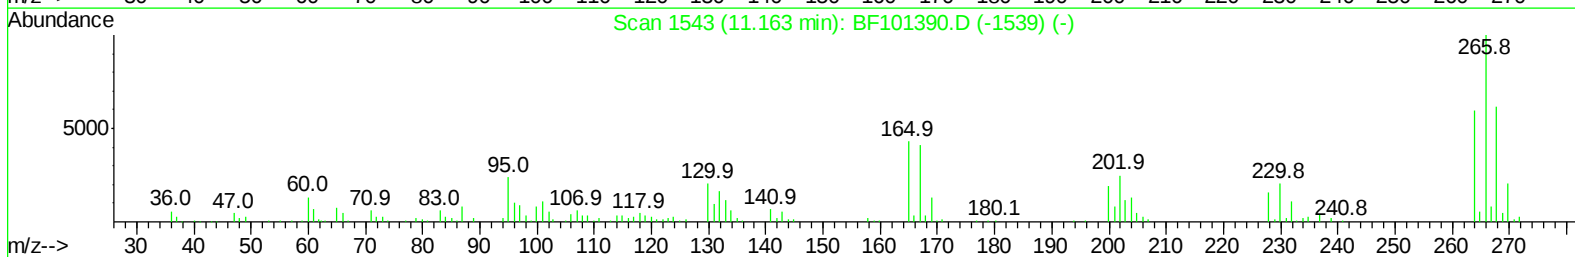
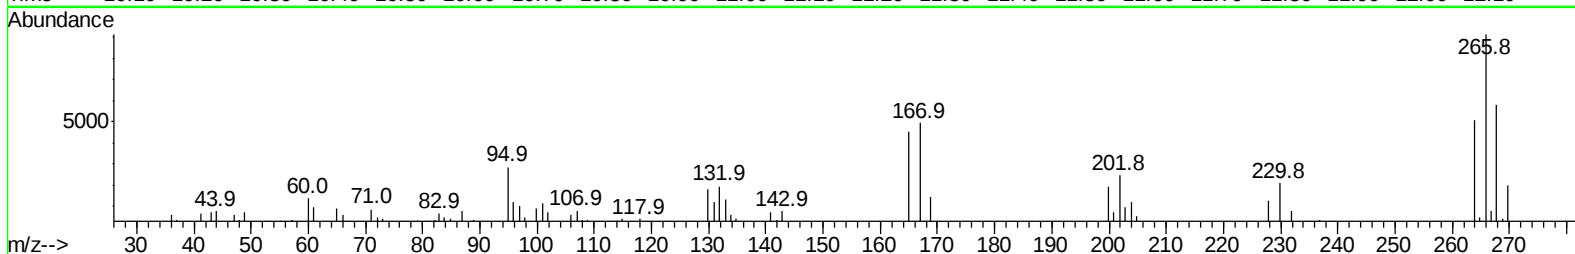


Data Path : U:\HPCHEM1\BNA F\DATA\BF010418\
Data File : BF101909.D
Acq On : 5 Jan 2018 00:24
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 05 06:58:01 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 04 14:22:17 2018
Response via : Initial Calibration

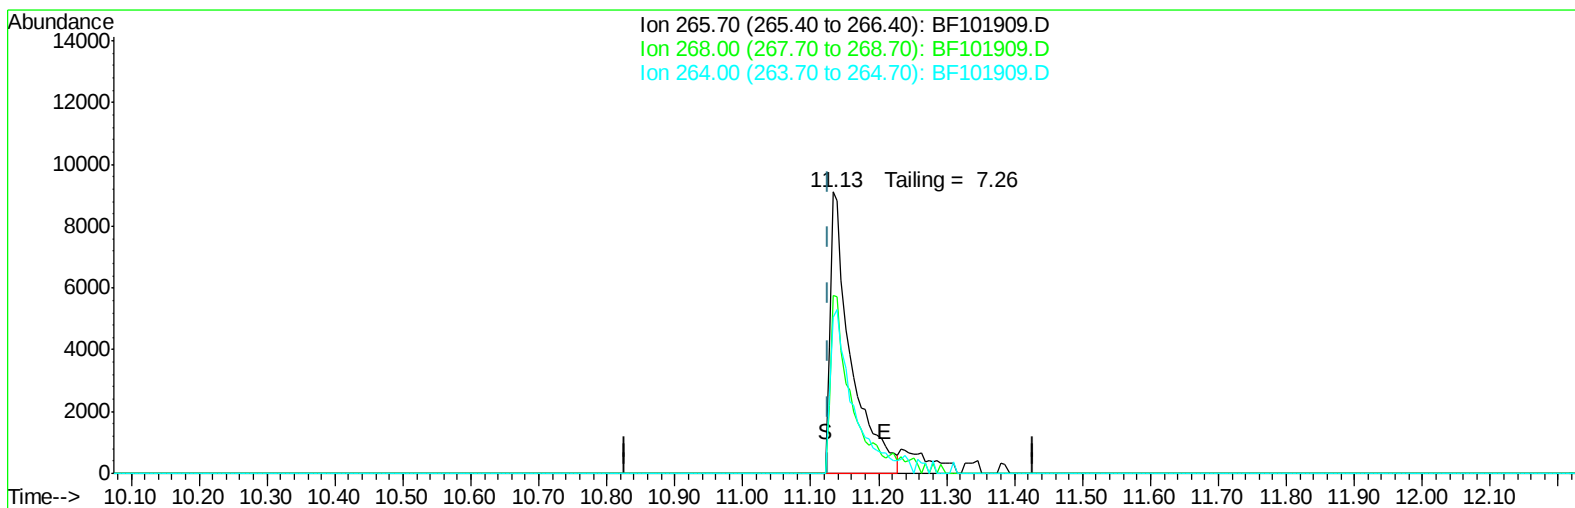

TIC: BF101909.D

(69) Pentachlorophenol (C)




11.133min (+0.006) 0.00ng

response 19260

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.37
264.00	61.90	55.39
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA F\DATA\BF010418\
 Data File : BF101909.D
 Acq On : 5 Jan 2018 00:24
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 05 06:58:01 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF121417.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 04 14:22:17 2018
 Response via : Initial Calibration

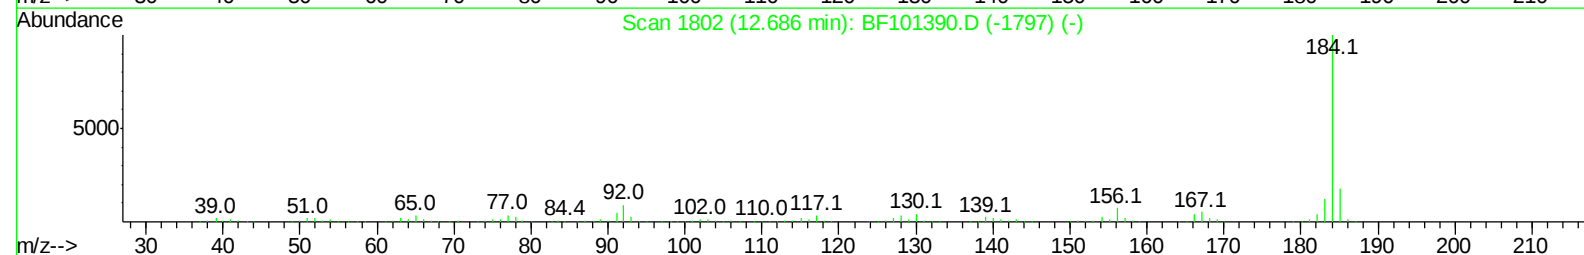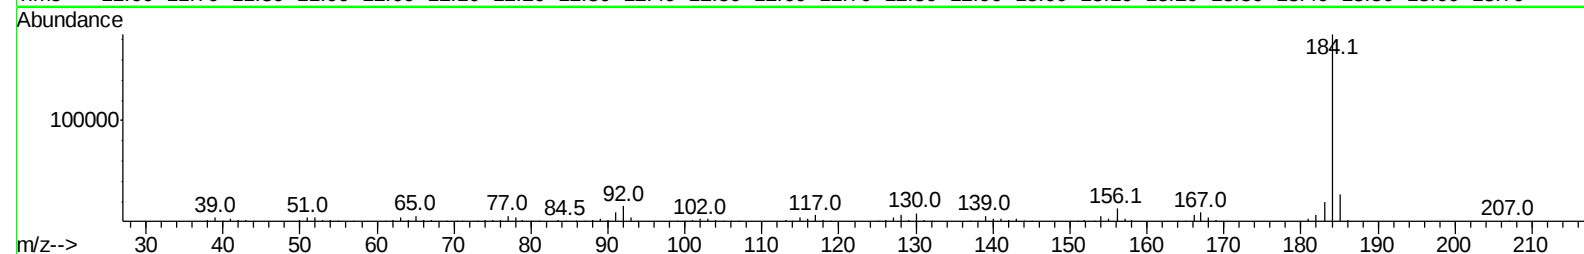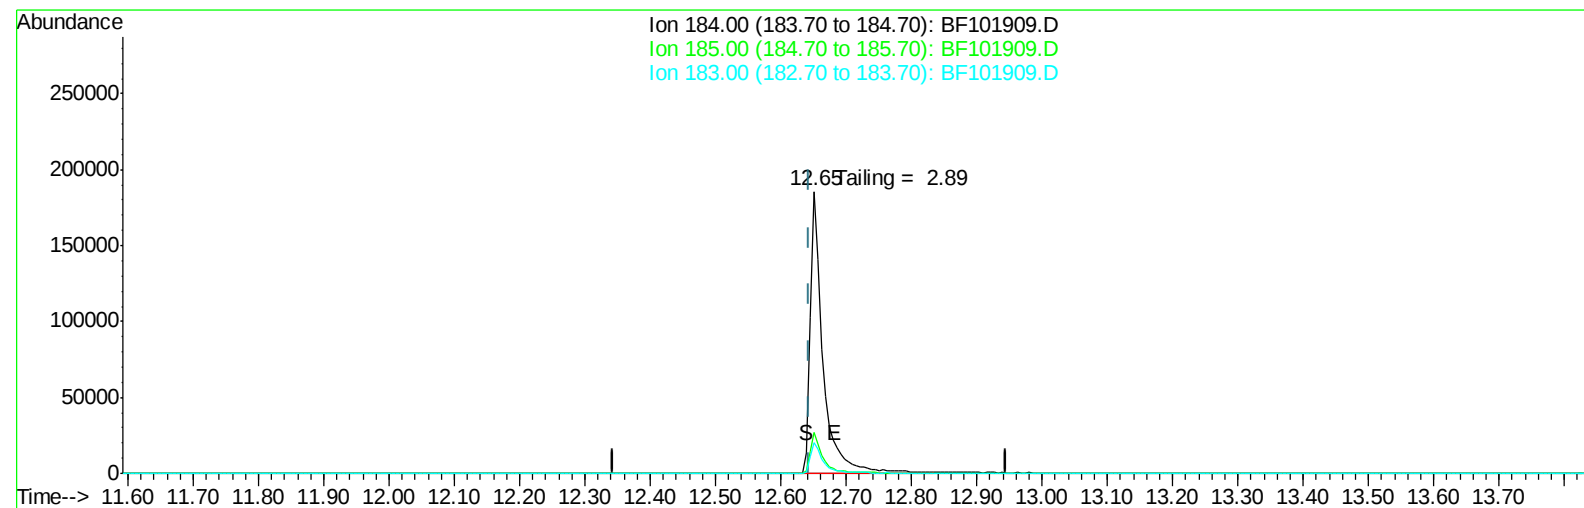

TIC: BF101909.D

(76) Benzidine

12.651min (+0.006) 46054.39ng

response 254810

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.34
183.00	11.60	10.72
0.00	0.00	0.00