


Data Path : Z:\HPCHEM1\BNA F\Data\BF010418\
 Data File : BF101885.D
 Acq On : 4 Jan 2018 12:26
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 05 12:29:26 2018

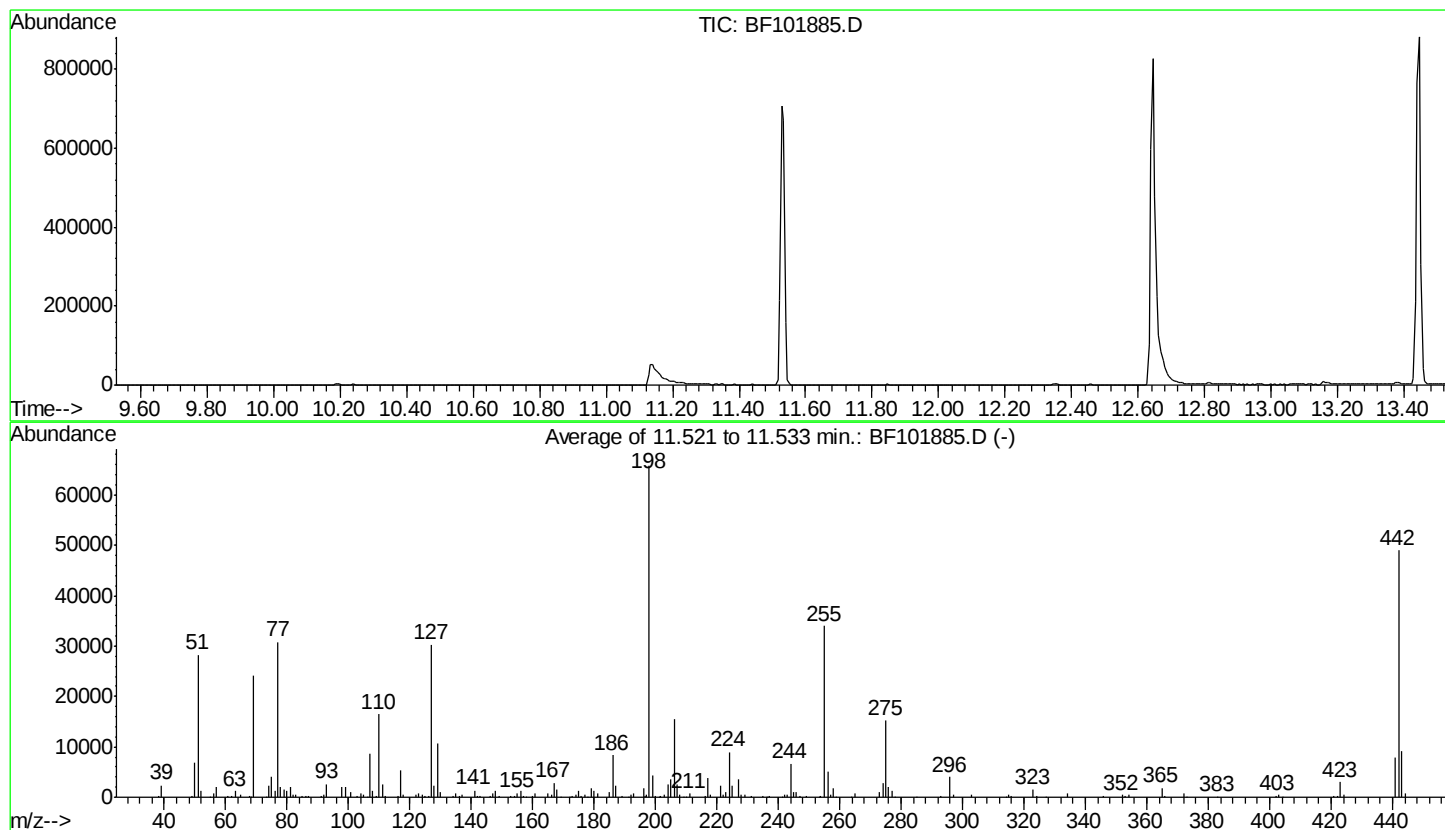

AutoFind: Scans 1604, 1605, 1606; Background Corrected with Scan 1600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.0	28312	PASS
68	69	0.00	2	0.9	210	PASS
69	198	0.00	100	36.5	24017	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.0	30237	PASS
197	198	0.00	2	0.8	510	PASS
198	198	100	100	100.0	65792	PASS
199	198	5	9	6.7	4378	PASS
275	198	10	60	23.1	15204	PASS
365	198	1	100	2.8	1829	PASS
441	443	0.01	100	86.8	7914	PASS
442	198	50	100	74.5	49002	PASS
443	442	15	24	18.6	9120	PASS