


Data Path : Z:\HPCHEM1\BNA F\Data\BF010418\
 Data File : BF101909.D
 Acq On : 5 Jan 2018 00:24
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF121417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 05 12:29:26 2018

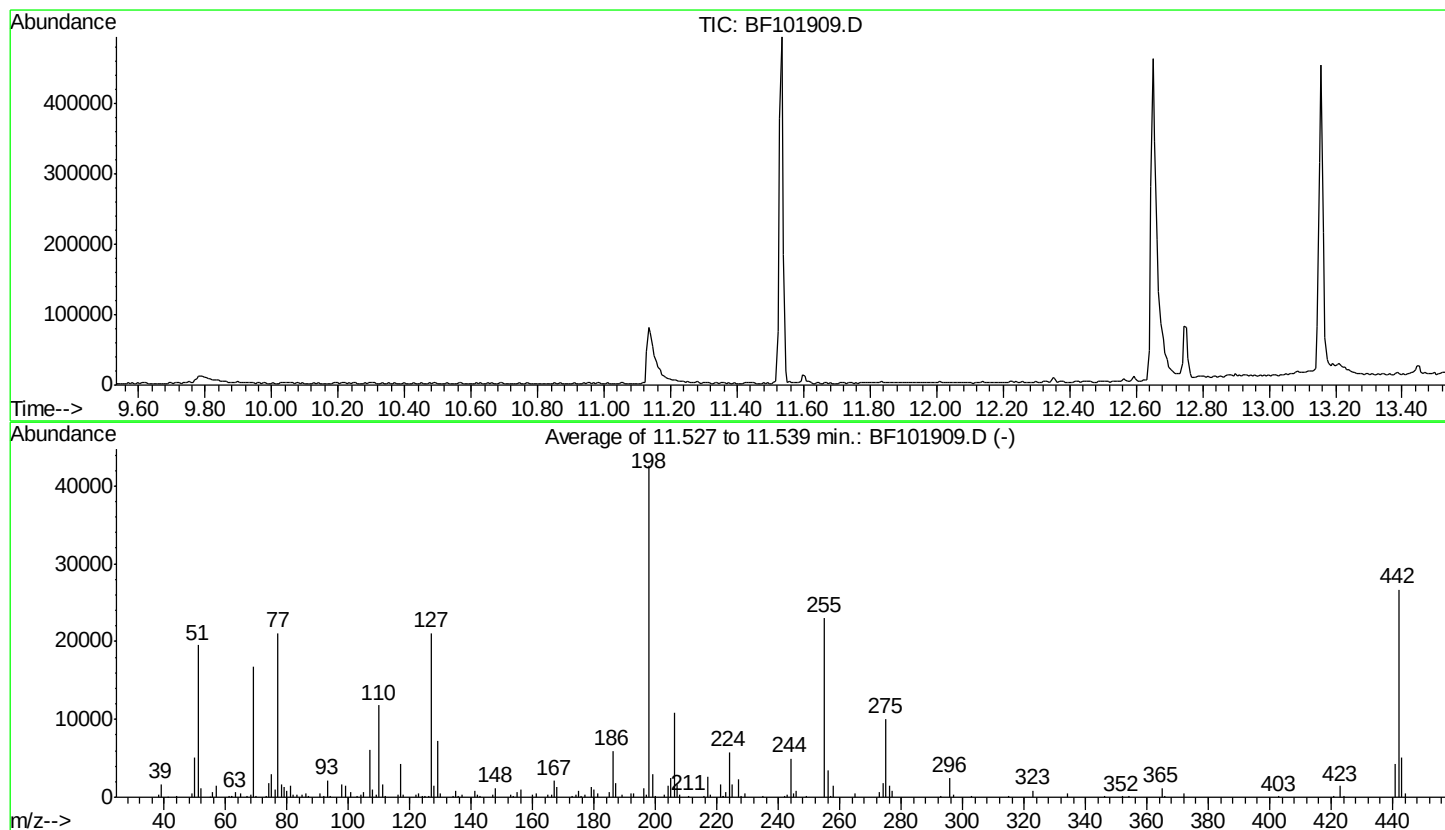

AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.9	19567	PASS
68	69	0.00	2	2.0	337	PASS
69	198	0.00	100	39.4	16797	PASS
70	69	0.00	2	0.6	100	PASS
127	198	10	80	49.5	21080	PASS
197	198	0.00	2	0.8	324	PASS
198	198	100	100	100.0	42610	PASS
199	198	5	9	6.8	2904	PASS
275	198	10	60	23.7	10103	PASS
365	198	1	100	2.8	1183	PASS
441	443	0.01	100	85.0	4269	PASS
442	198	50	100	62.7	26733	PASS
443	442	15	24	18.8	5022	PASS