
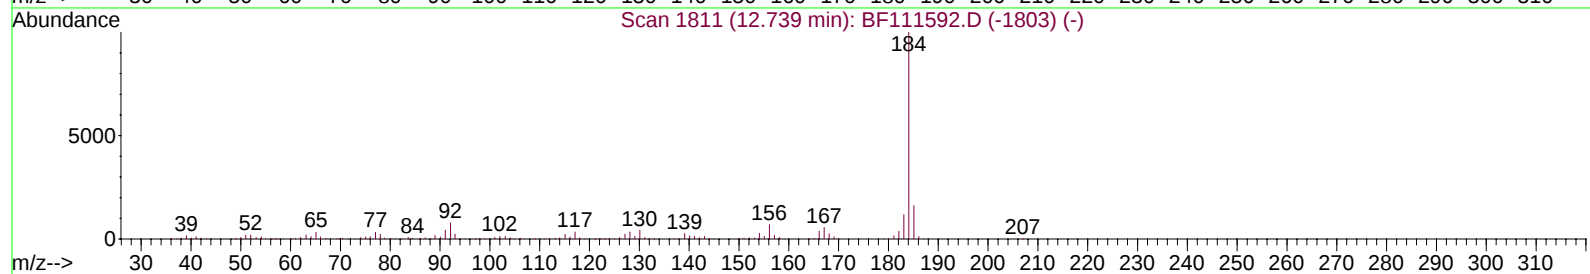
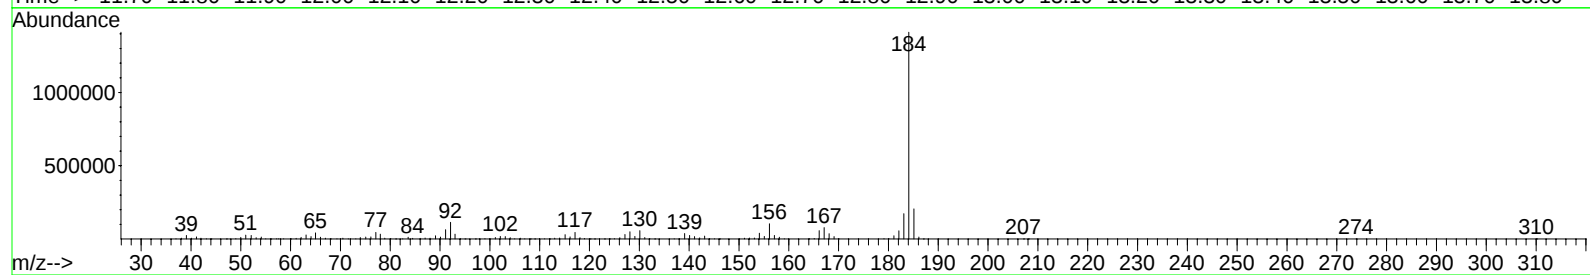


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF010419\
 Data File : BF111841.D
 Acq On : 4 Jan 2019 13:38
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 04 16:21:40 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF121918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 19 17:39:39 2018
 Response via : Initial Calibration

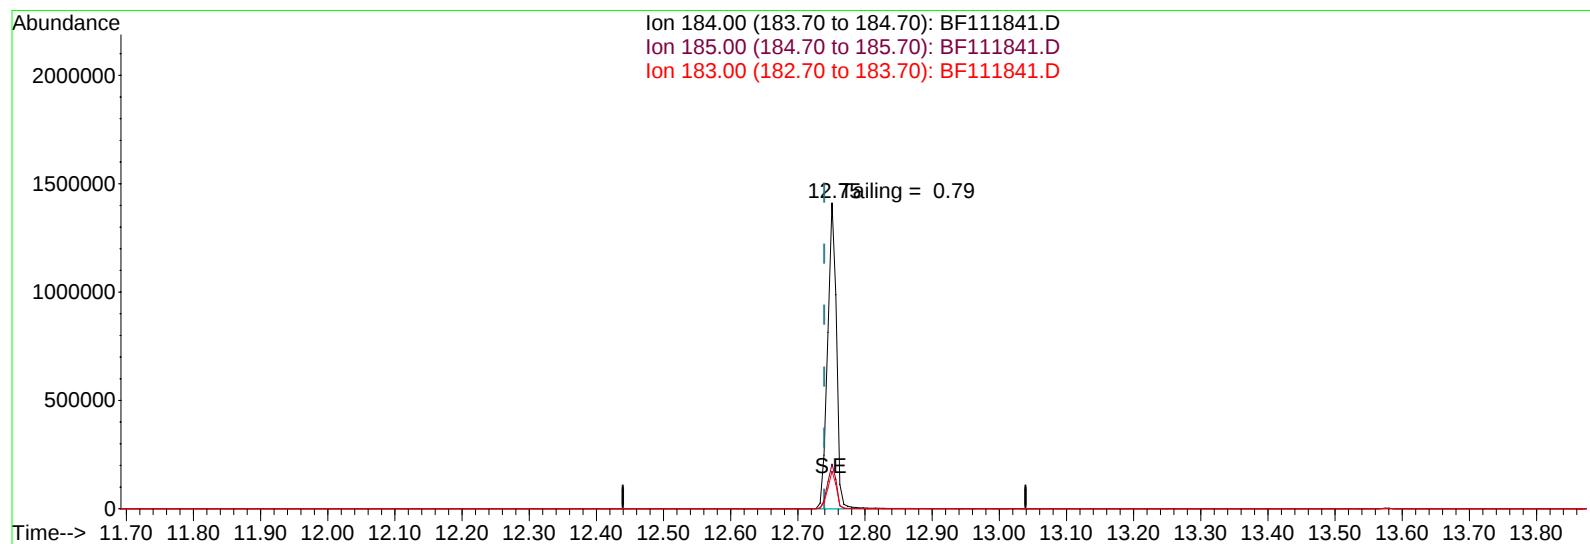

TIC: BF111841.D

(77) Benzidine




12.751min (+0.012) 0.00ng

response 1298462

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.61
183.00	11.60	12.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF010419\
Data File : BF111841.D
Acq On : 4 Jan 2019 13:38
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 04 16:21:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF121918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 17:39:39 2018
Response via : Initial Calibration

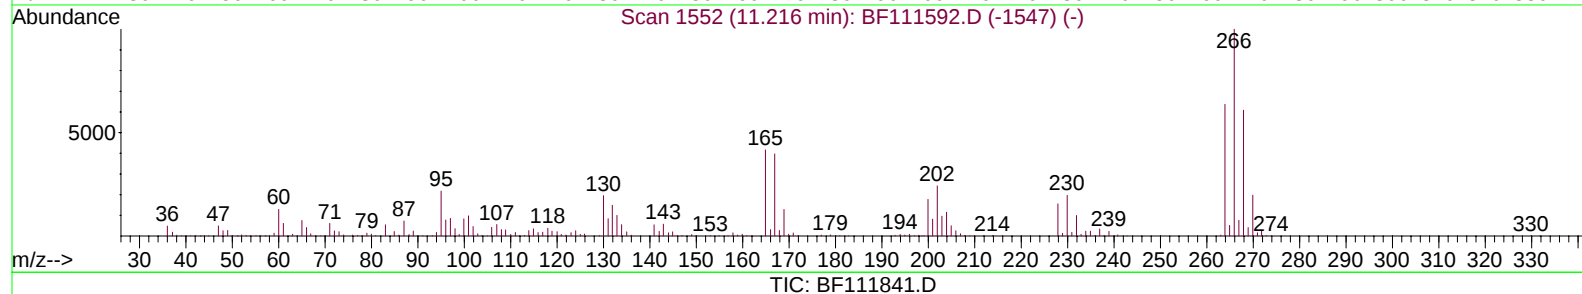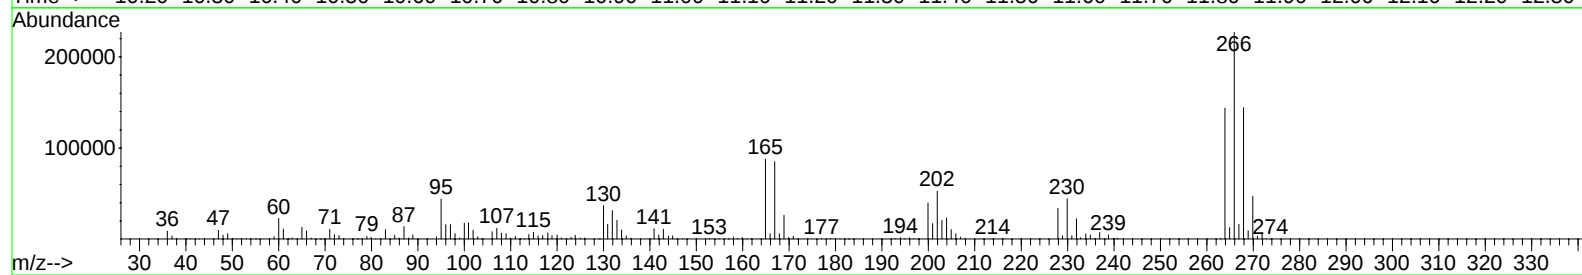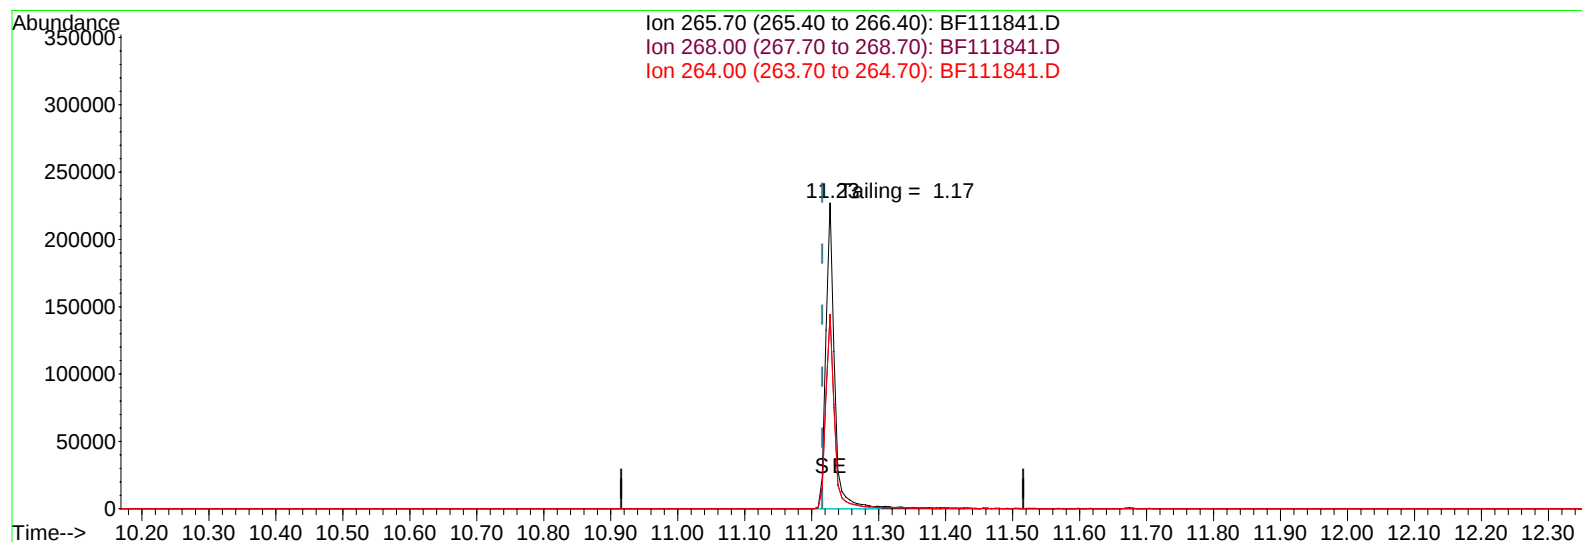

(70) Pentachlorophenol (C)

11.227min (+0.012) 30489.00ng

response 207750

Ion	Exp%	Act%
265.70	100	100
268.00	59.90	63.56
264.00	61.40	63.39
0.00	0.00	0.00