


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF010419\
 Data File : BF111841.D
 Acq On : 4 Jan 2019 13:38
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 19 17:39:39 2018

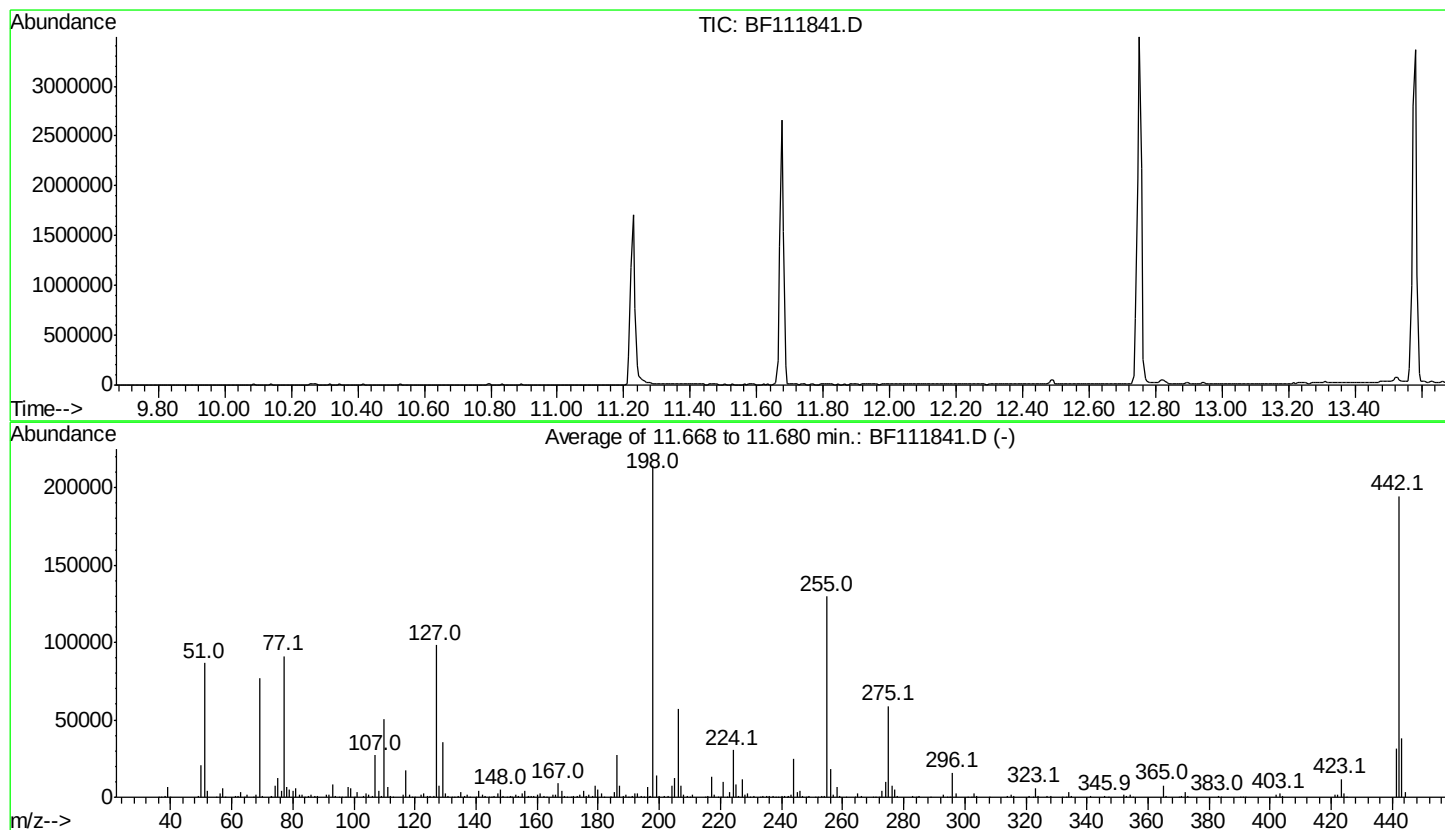

AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1624

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.4	86463	PASS
68	69	0.00	2	1.8	1362	PASS
69	198	0.00	100	36.1	77312	PASS
70	69	0.00	2	0.6	470	PASS
127	198	10	80	45.9	98277	PASS
197	198	0.00	2	0.6	1229	PASS
198	198	100	100	100.0	214186	PASS
199	198	5	9	6.7	14319	PASS
275	198	10	60	27.5	59000	PASS
365	198	1	100	3.6	7655	PASS
441	198	0.01	100	14.7	31406	PASS
442	198	50	100	90.9	194648	PASS
443	442	15	24	19.6	38126	PASS