
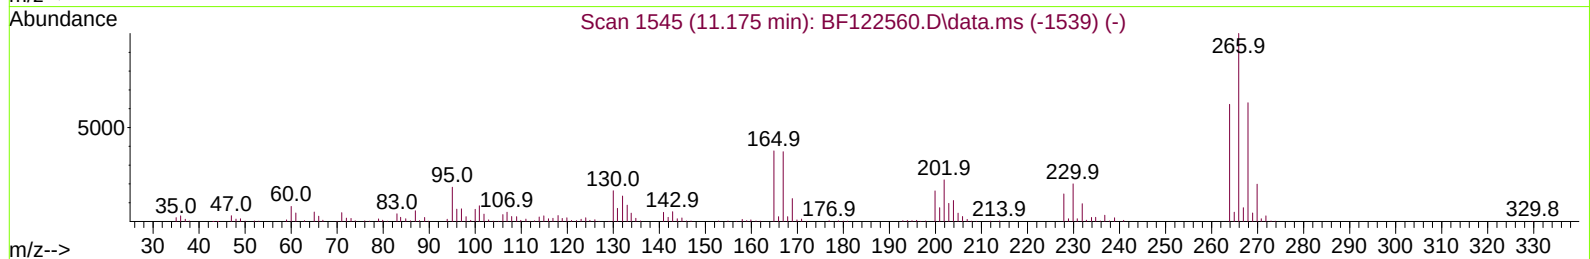
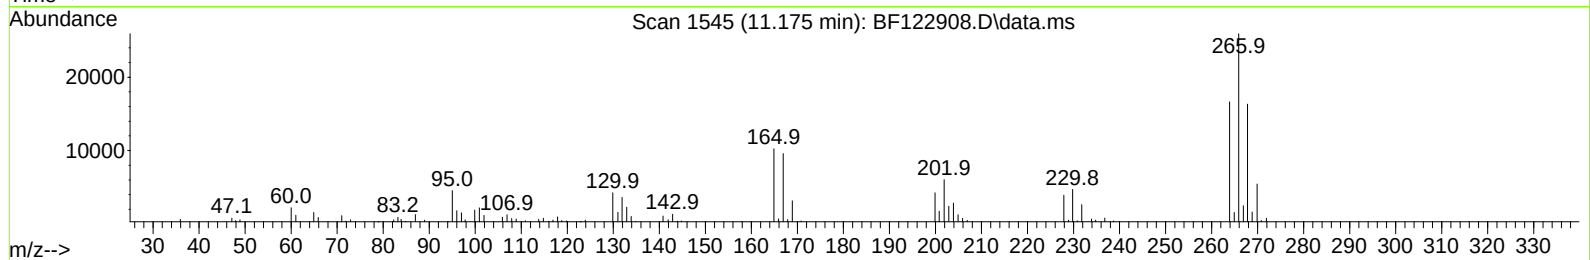


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010421\
Data File : BF122908.D
Acq On : 4 Jan 2021 12:58
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 05 00:34:35 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 31 15:53:00 2020
Response via : Initial Calibration

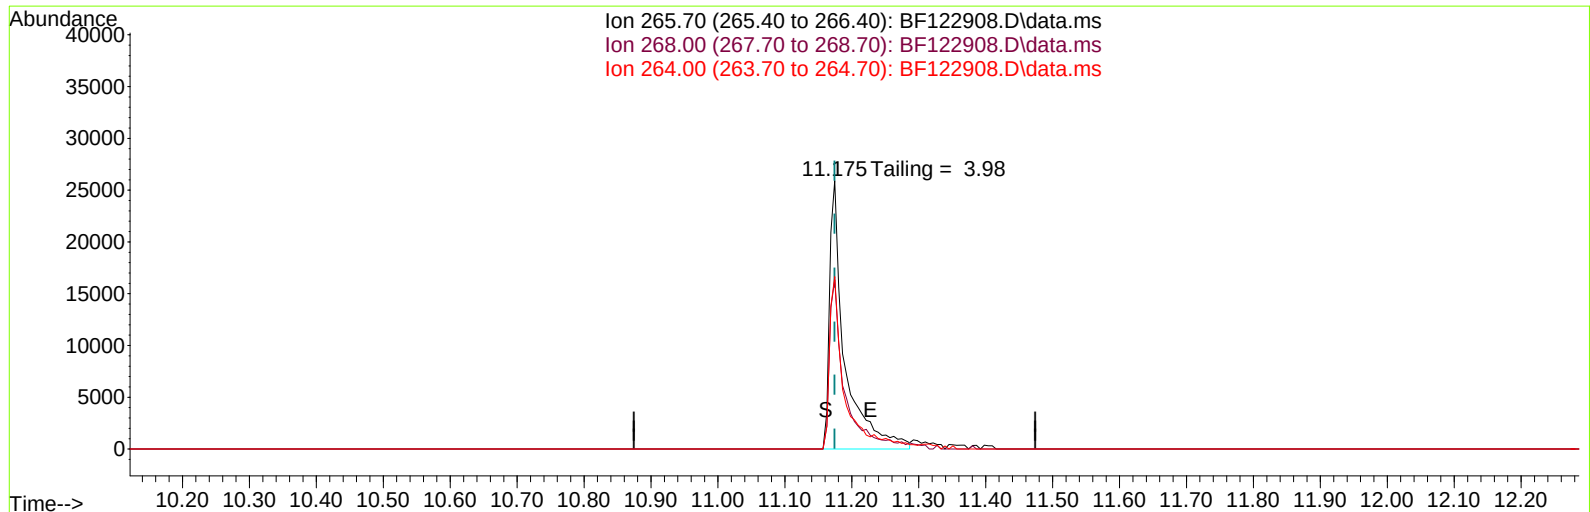

TIC: BF122908.D\data.ms

(70) Pentachlorophenol (C)




11.175min (+ 0.000) 0.00 ng

response 41212

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.02
264.00	62.30	64.20
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010421\  
Data File : BF122908.D  
Acq On    : 4 Jan 2021 12:58  
Operator  : JU/CG  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1 Sample Multiplier: 1
```

Quant Time: Jan 05 00:34:35 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 31 15:53:00 2020
Response via : Initial Calibration

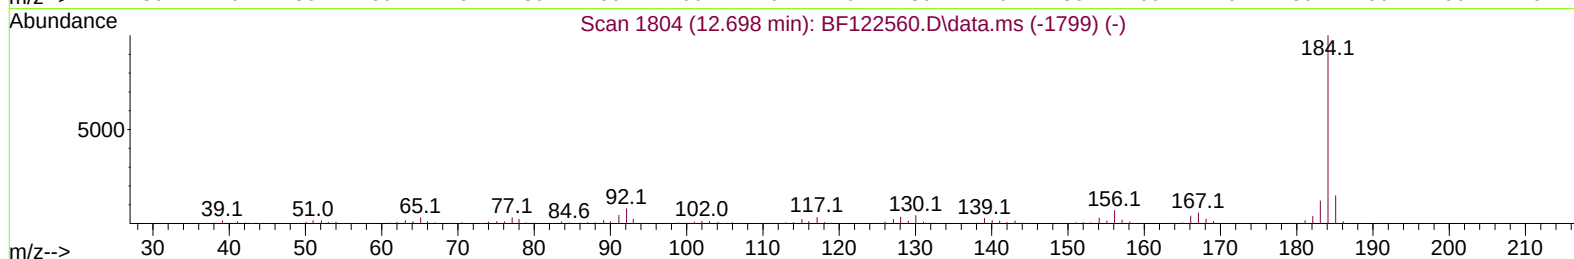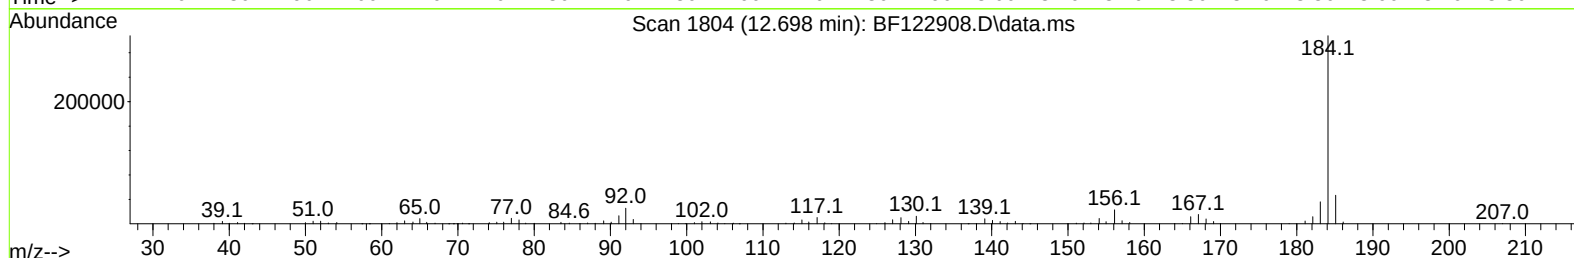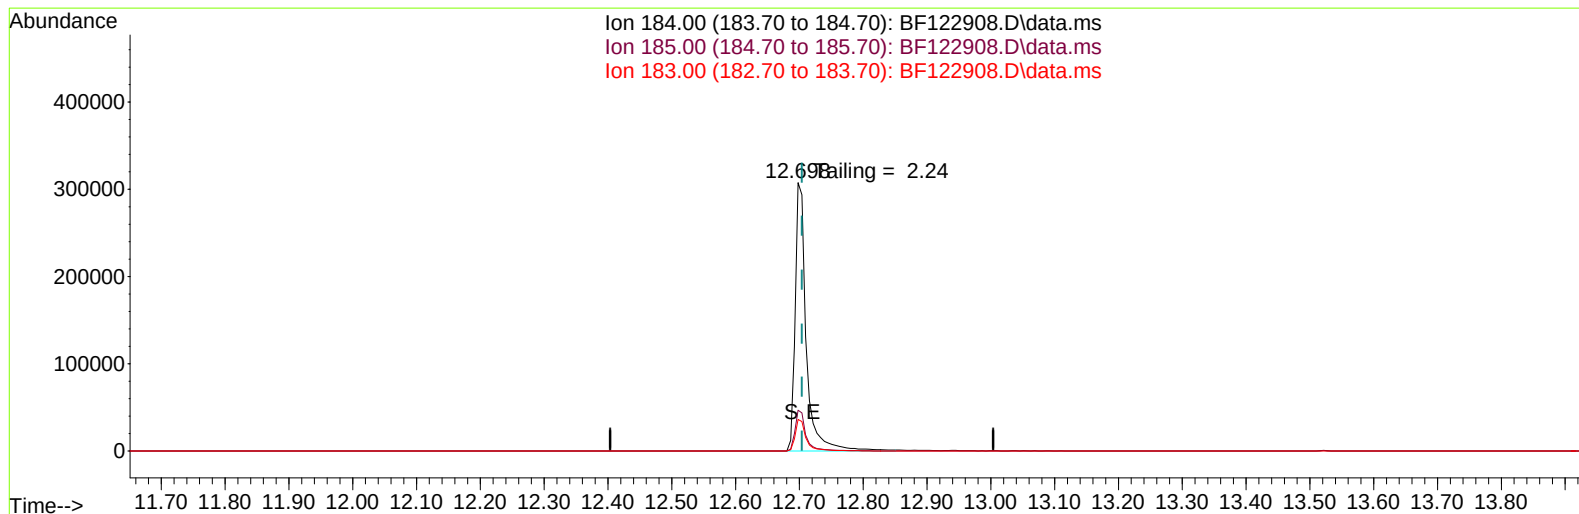

TIC: BF122908.D\data.ms

(77) Benzidine

12.698min (-0.006) 0.00 ng

response **378087**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	15.21
183.00	12.10	11.79
0.00	0.00	0.00