


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010421\
 Data File : BF122908.D
 Acq On : 4 Jan 2021 12:58
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 31 15:53:00 2020

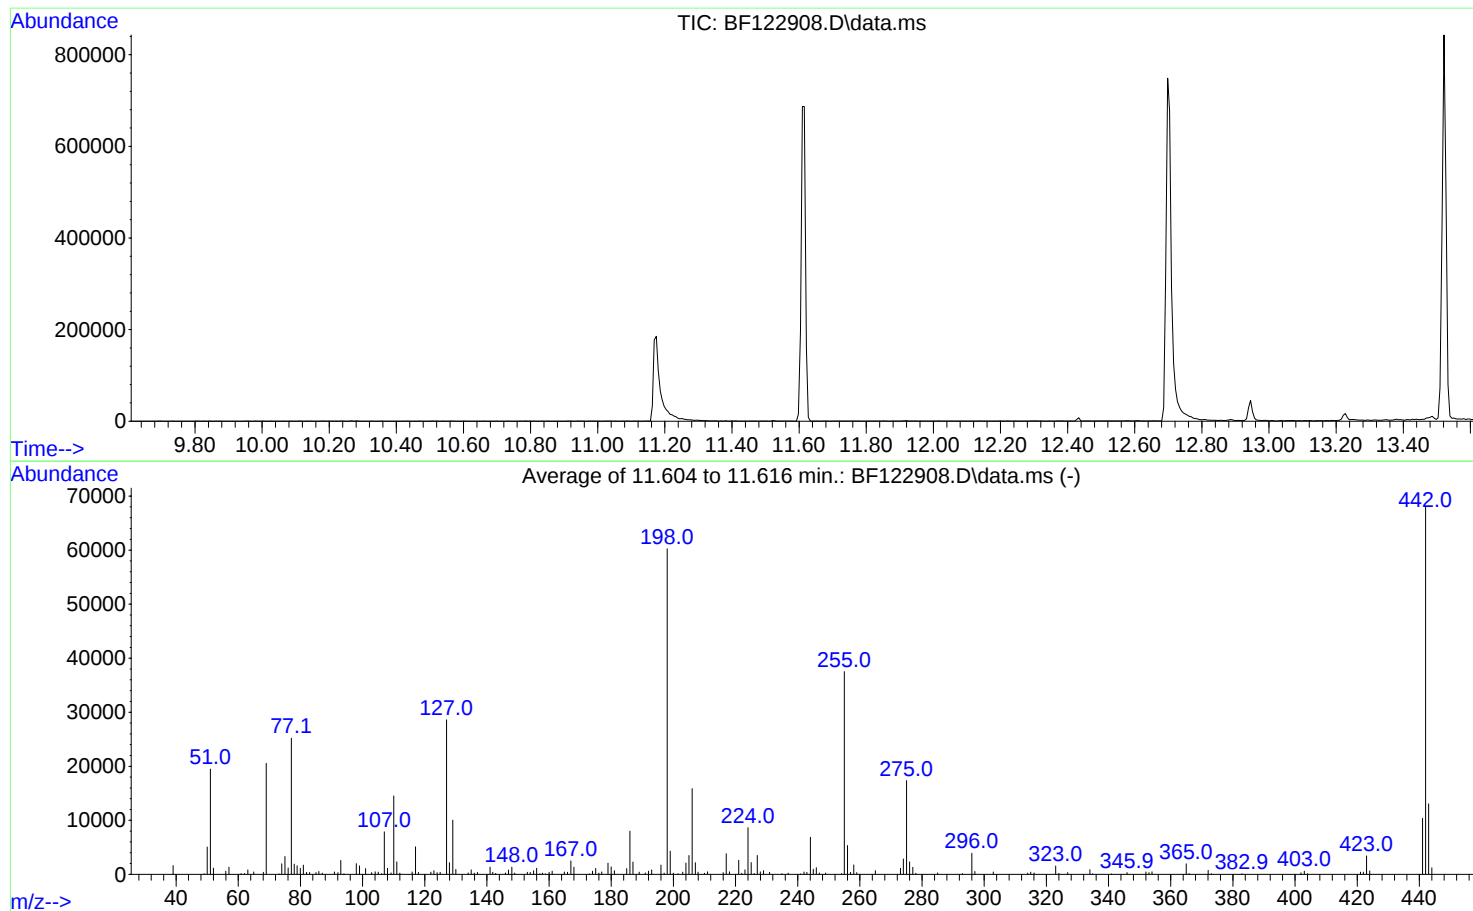

AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.3	19492	PASS
68	69	0.00	2	1.9	391	PASS
69	198	0.00	100	34.1	20563	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.5	28617	PASS
197	198	0.00	2	0.4	226	PASS
198	198	100	100	100.0	60264	PASS
199	198	5	9	7.1	4281	PASS
275	198	10	60	28.8	17340	PASS
365	198	1	100	3.2	1957	PASS
441	198	0.01	100	17.2	10376	PASS
442	442	100	100	100.0	68074	PASS
443	442	15	24	19.2	13053	PASS