


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010422\
 Data File : BF126467.D
 Acq On : 4 Jan 2022 14:39
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 05 01:57:07 2022

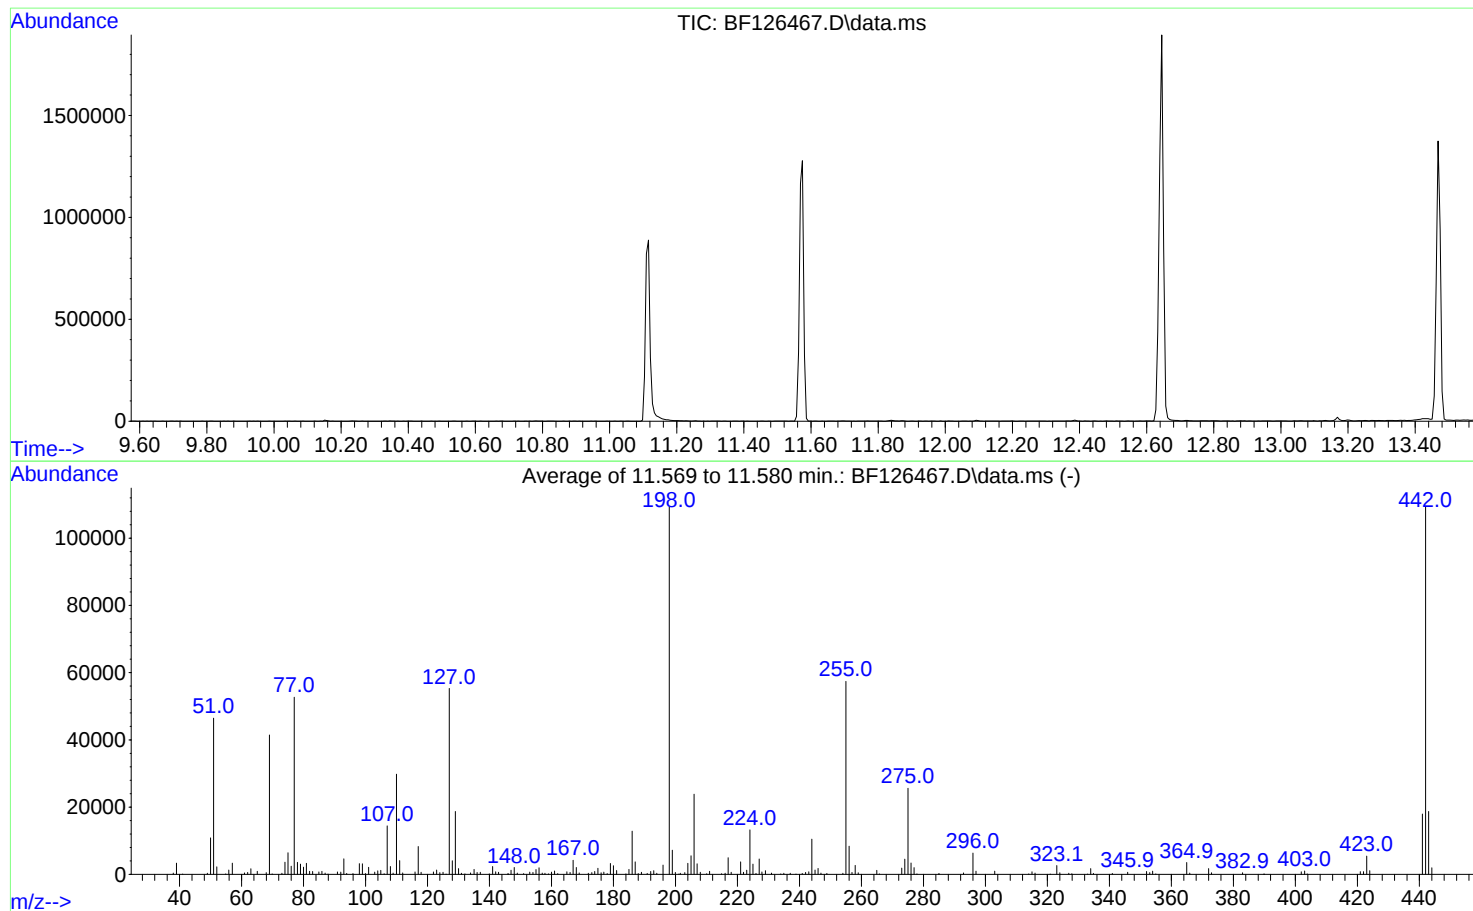




AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.5	46439	PASS
68	69	0.00	2	1.2	515	PASS
69	198	0.00	100	37.9	41441	PASS
70	69	0.00	2	0.3	137	PASS
127	198	10	80	50.6	55293	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	109277	PASS
199	198	5	9	6.6	7181	PASS
275	198	10	60	23.4	25616	PASS
365	198	1	100	3.2	3544	PASS
441	198	0.01	100	16.4	17958	PASS
442	442	50	100	100.0	109411	PASS
443	442	15	24	17.1	18689	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010422\
Data File : BF126467.D
Acq On : 4 Jan 2022 14:39
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 05 03:15:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 05 01:57:07 2022
Response via : Initial Calibration

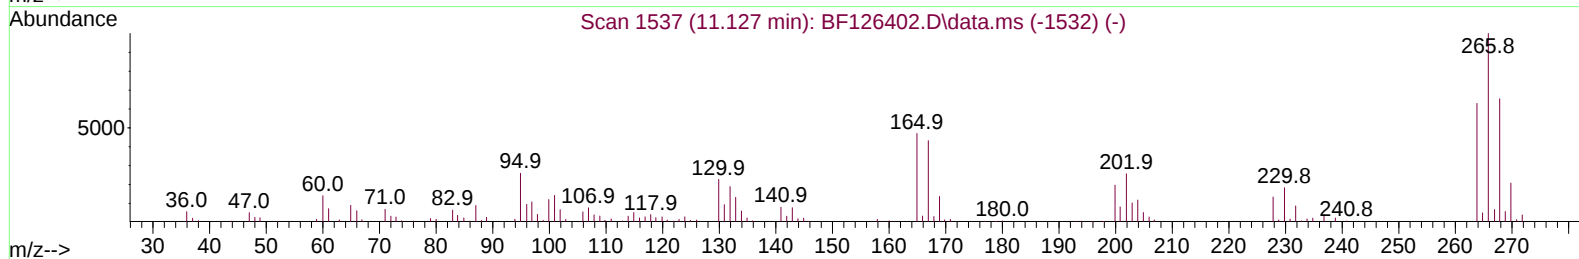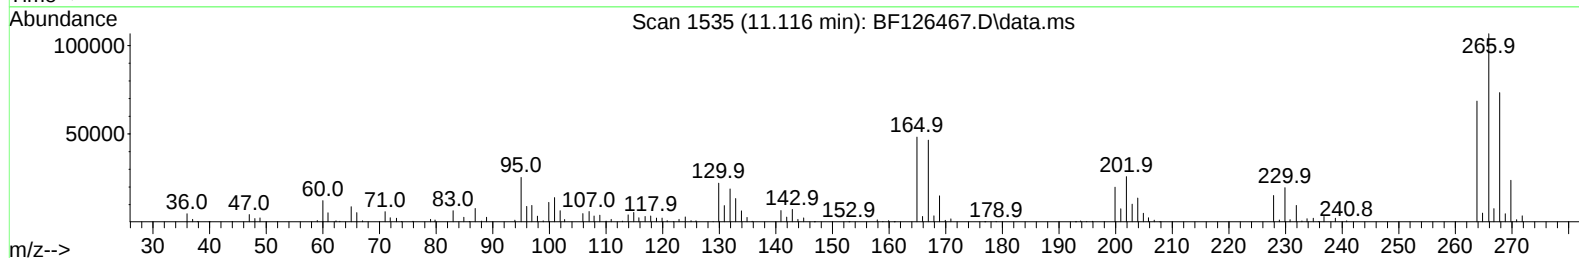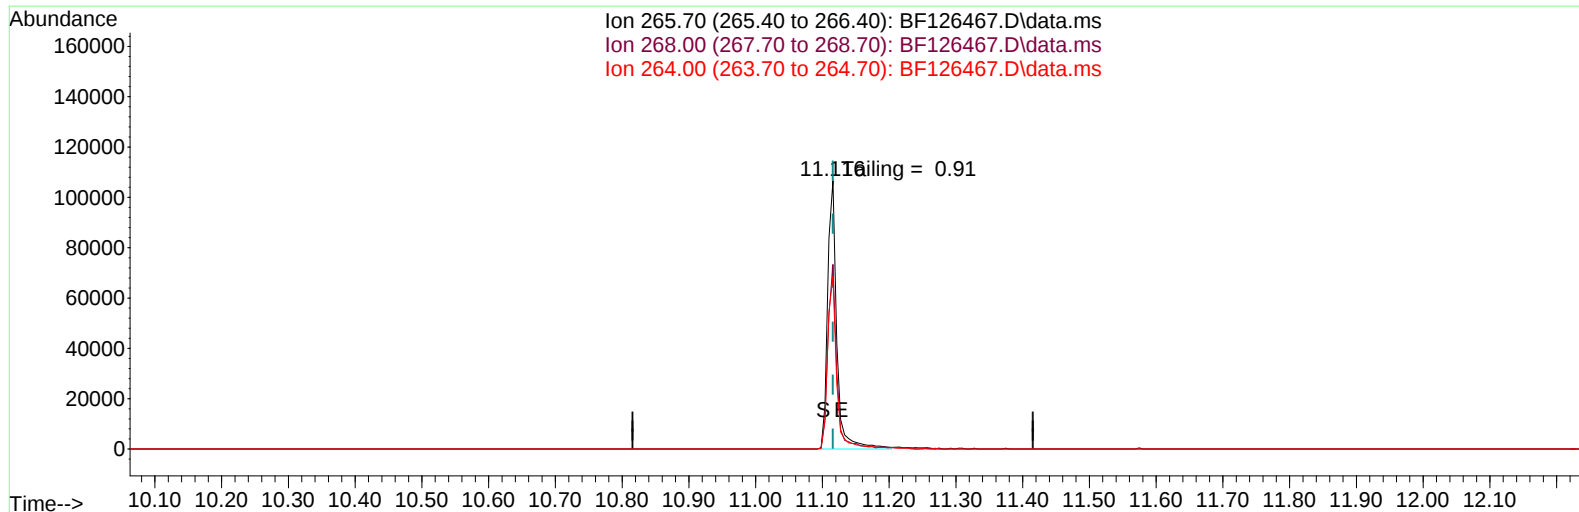

TIC: BF126467.D\data.ms

(70) Pentachlorophenol (C)

11.116min (+ 0.000) 76632.62 ng

response 103058

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	68.74
264.00	63.00	64.32
0.00	0.00	0.00

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/4/2022	BNA_F	<u>BF126467.D</u>
Compound Name	Response	Retention Time
DDT	222239	13.468
DDD	4490	13.168
DDE	0	12.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4490	226729	1.98