


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010423\
 Data File : BF131893.D
 Acq On : 04 Jan 2023 11:42
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 30 02:06:40 2022

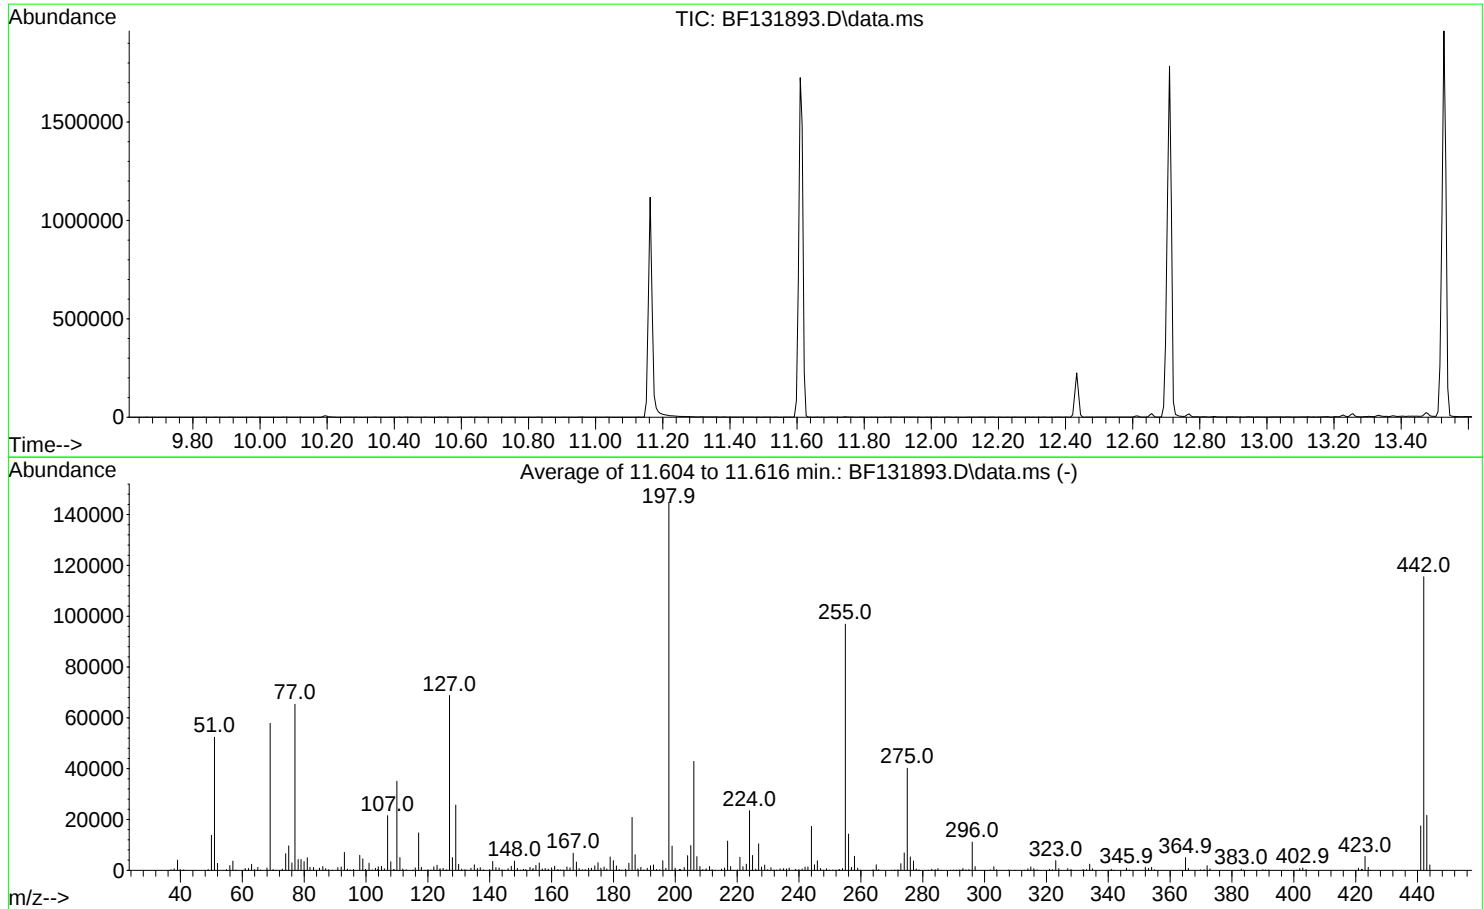




AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1613

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	52352	PASS
68	69	0.00	2	1.6	932	PASS
69	198	0.00	100	39.9	57840	PASS
70	69	0.00	2	0.2	140	PASS
127	198	10	80	47.5	68827	PASS
197	198	0.00	2	0.6	812	PASS
198	198	100	100	100.0	144787	PASS
199	198	5	9	6.6	9557	PASS
275	198	10	60	27.7	40173	PASS
365	198	1	100	3.4	4985	PASS
441	198	0.01	100	12.1	17452	PASS
442	442	50	100	100.0	115560	PASS
443	442	15	24	18.7	21614	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010423\
Data File : BF131893.D
Acq On : 04 Jan 2023 11:42
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 05 07:25:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 30 02:06:40 2022
Response via : Initial Calibration

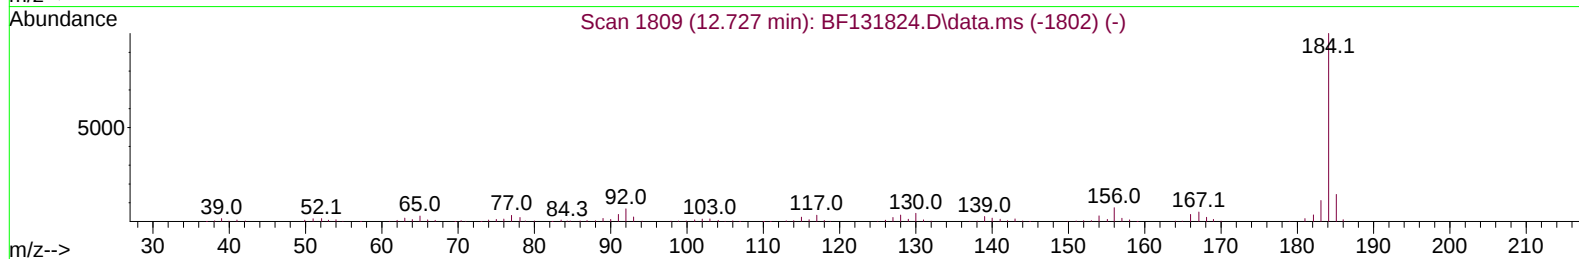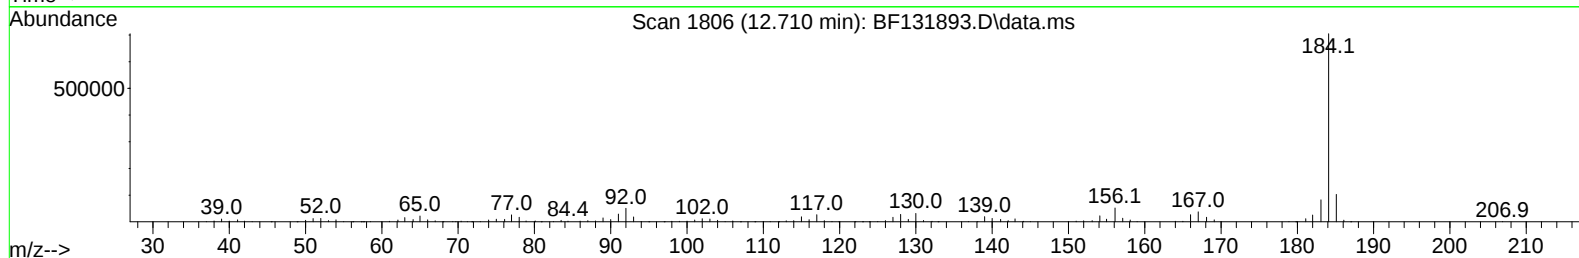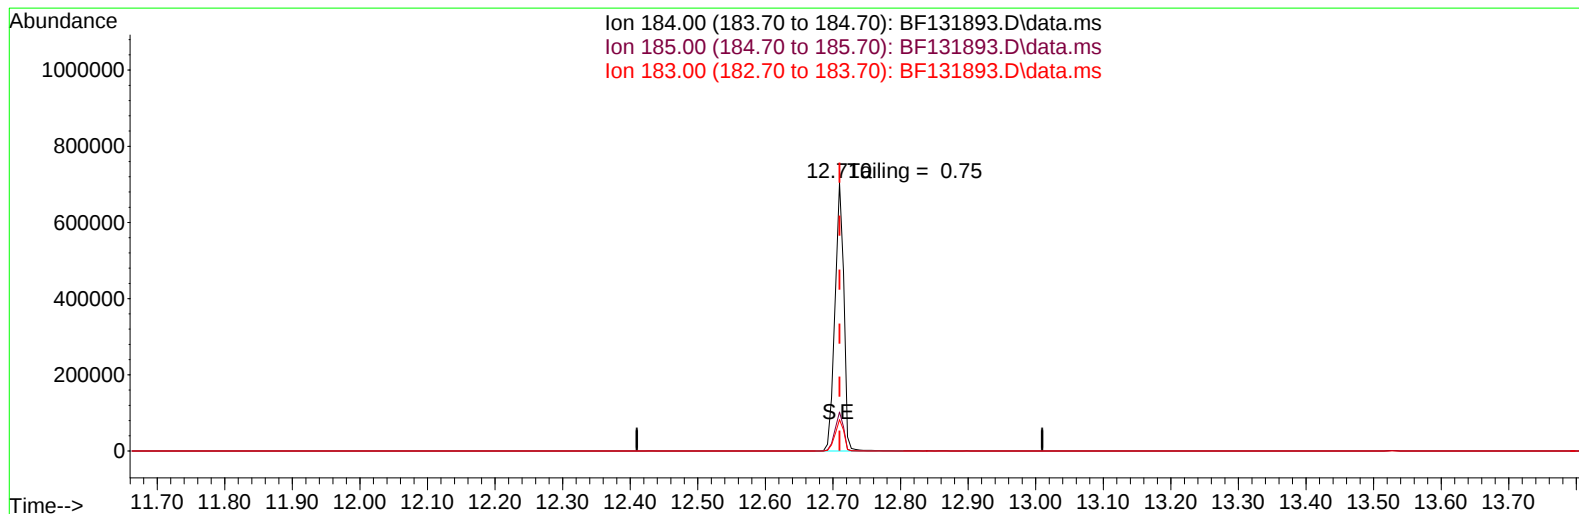

TIC: BF131893.D\data.ms

(77) Benzidine

12.710min (-0.000) 235982.38 ng

response 639879

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.56
183.00	11.20	11.67
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/4/2023	BNA_F	<u>BF131893.D</u>
Compound Name	Response	Retention Time
DDT	324388	13.527
DDD	5230	13.257
DDE	315	12.886
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5545	329933	1.68

Instrument :
BNA_F
ClientSampleId :
DFTPP