
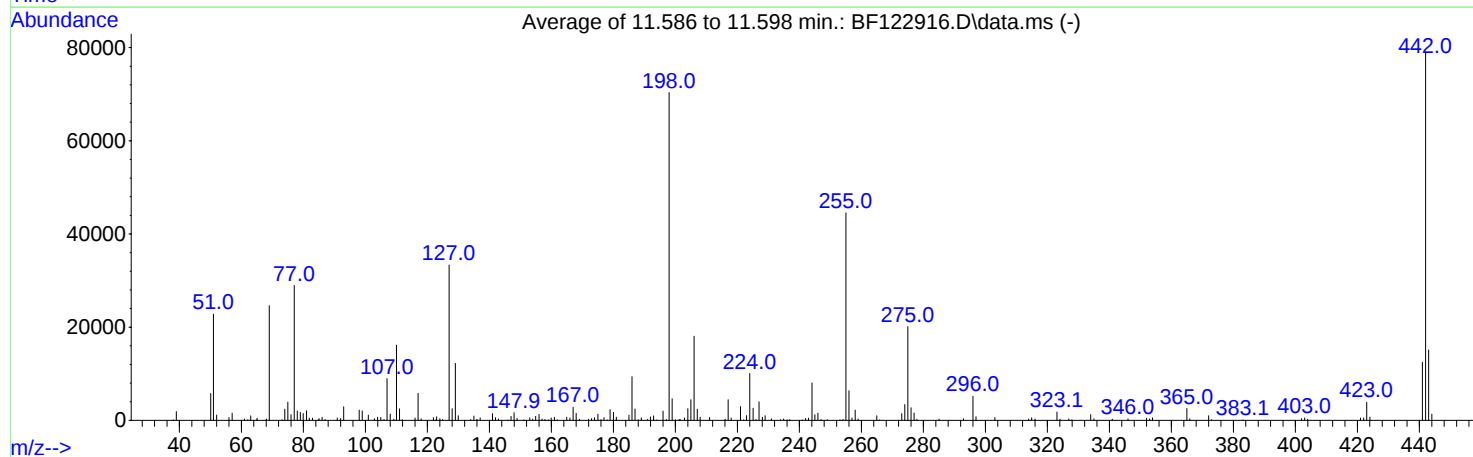


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010521\
 Data File : BF122916.D
 Acq On : 5 Jan 2021 11:36
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF010521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 05 16:45:30 2021

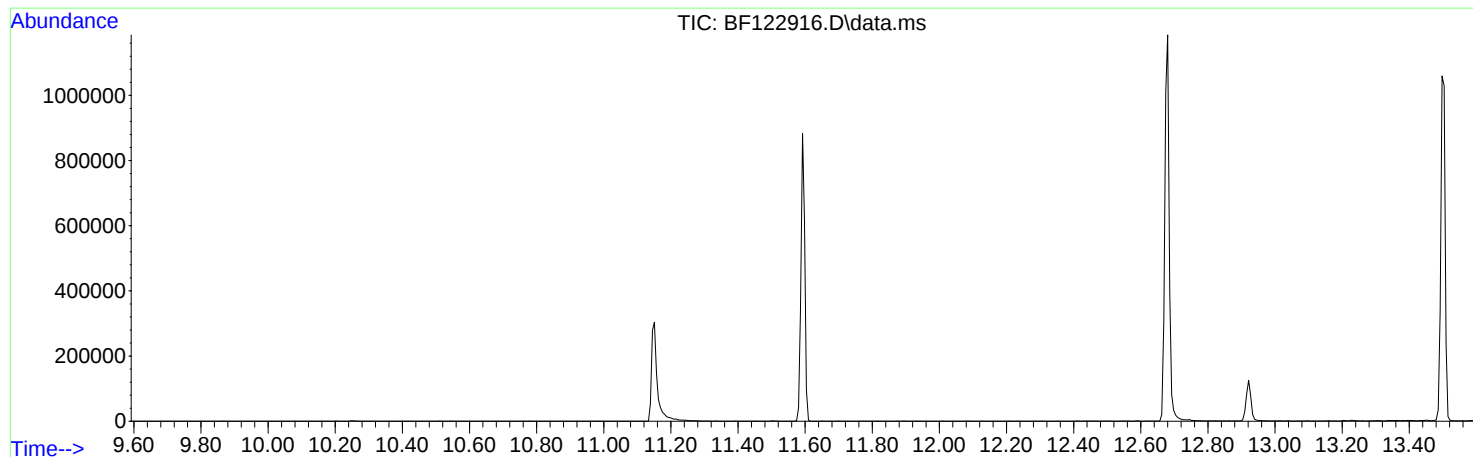

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.4	22819	PASS
68	69	0.00	2	1.3	313	PASS
69	198	0.00	100	35.0	24619	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.4	33357	PASS
197	198	0.00	2	0.3	191	PASS
198	198	100	100	100.0	70368	PASS
199	198	5	9	6.6	4626	PASS
275	198	10	60	28.6	20121	PASS
365	198	1	100	3.6	2557	PASS
441	198	0.01	100	17.7	12478	PASS
442	442	100	100	100.0	78952	PASS
443	442	15	24	19.1	15099	PASS