
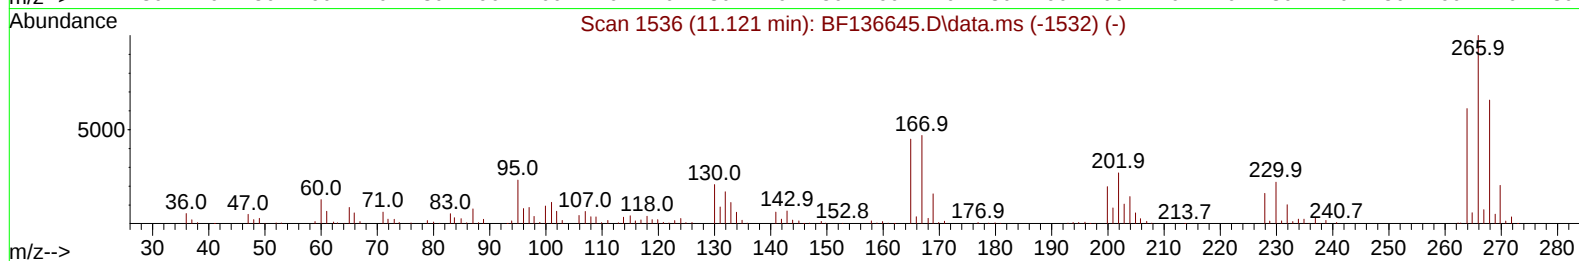
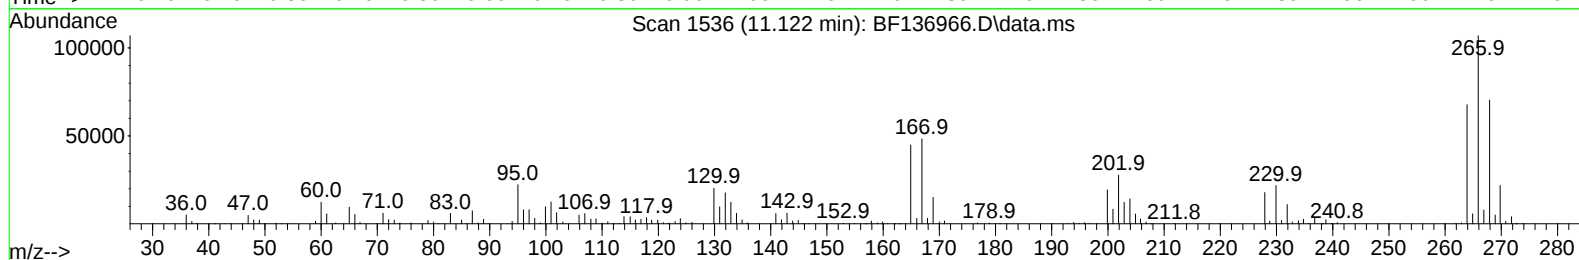


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010524\
Data File : BF136966.D
Acq On : 05 Jan 2024 09:45
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 05 11:00:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

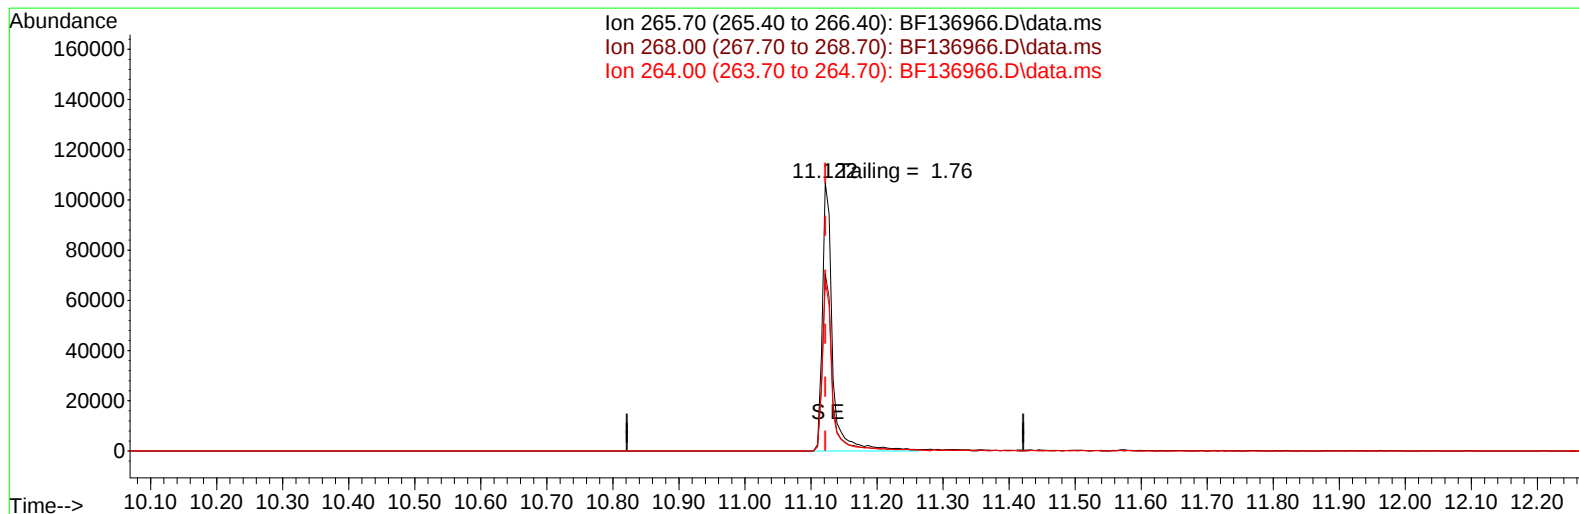

TIC: BF136966.D\data.ms

(70) Pentachlorophenol (C)




11.122min (+ 0.000) 29818.58 ng

response 114563

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	65.87
264.00	61.20	63.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010524\
Data File : BF136966.D
Acq On : 05 Jan 2024 09:45
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 05 11:00:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

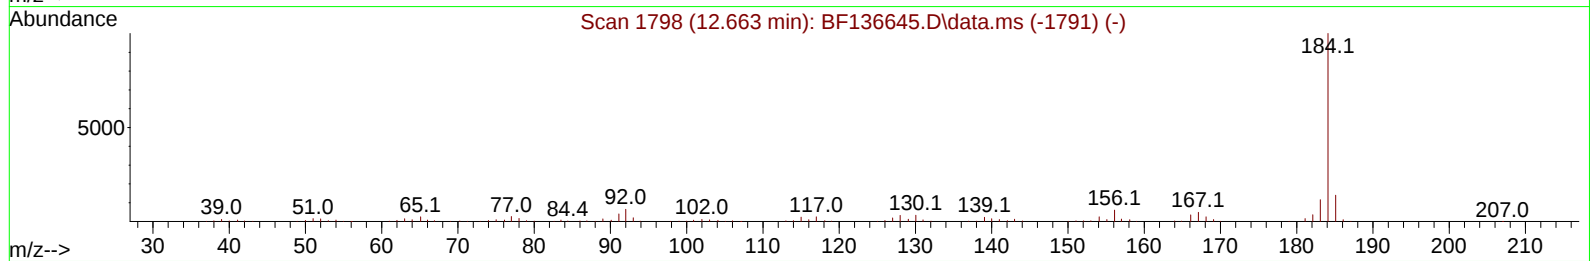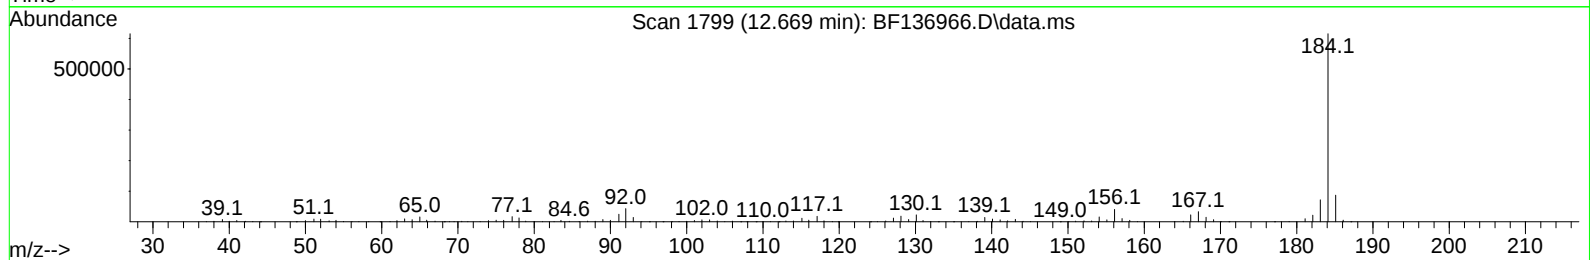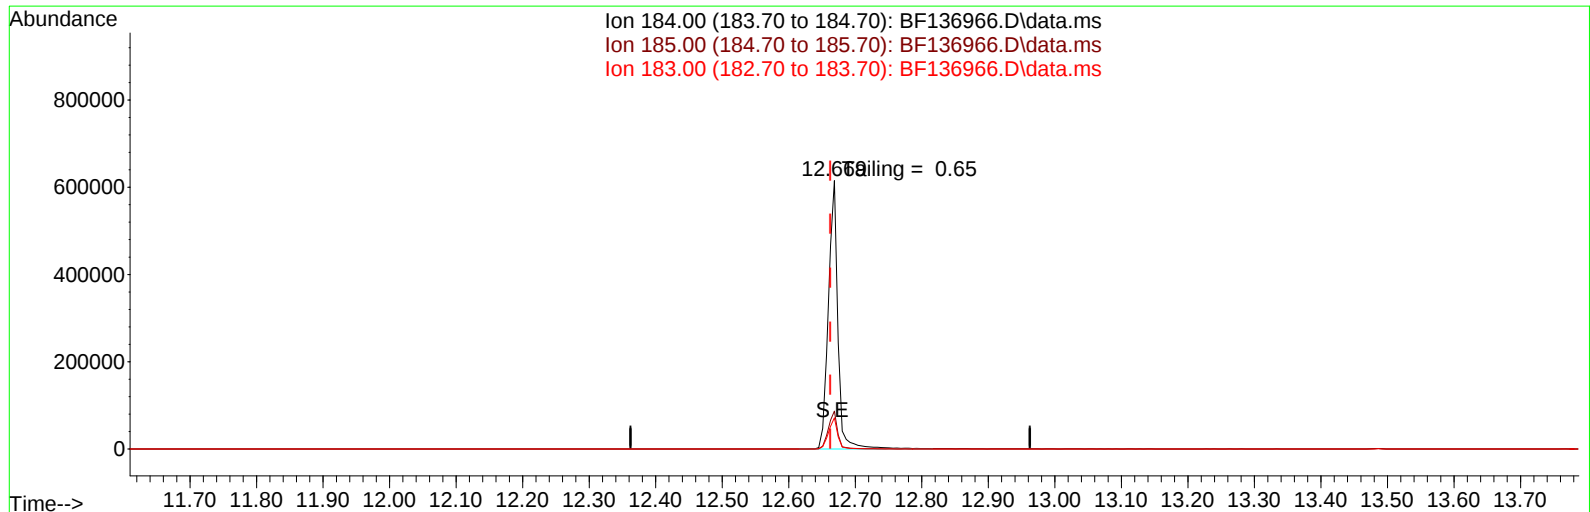

TIC: BF136966.D\data.ms

(77) Benzidine

12.669min (+ 0.006) 320372.05 ng m

response 614016

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.14
183.00	11.60	11.67
0.00	0.00	0.00