
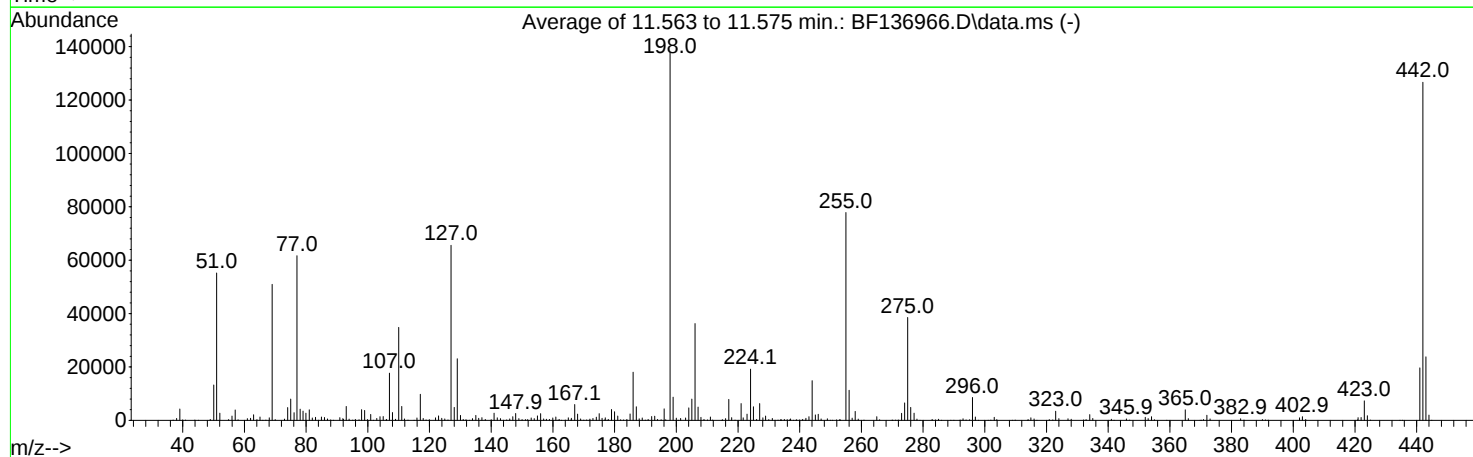


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010524\
Data File : BF136966.D
Acq On : 05 Jan 2024 09:45
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 21 01:54:25 2023

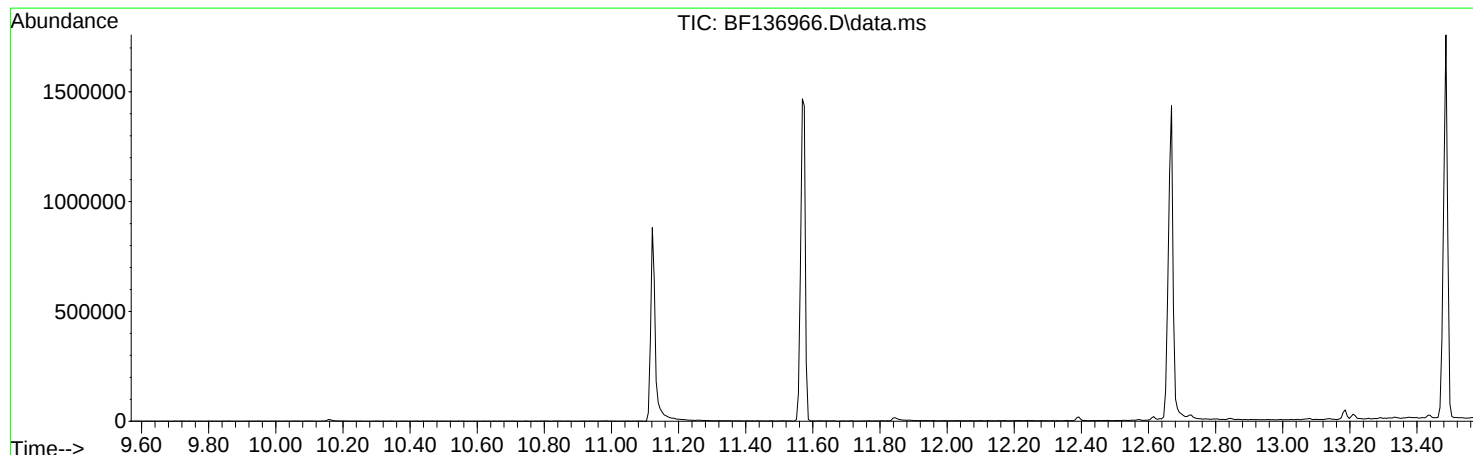

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.1	55213	PASS
68	69	0.00	2	1.9	982	PASS
69	198	0.00	100	37.0	50955	PASS
70	69	0.00	2	0.6	324	PASS
127	198	10	80	47.6	65584	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	137808	PASS
199	198	5	9	6.3	8673	PASS
275	198	10	60	28.0	38573	PASS
365	198	1	100	2.9	3971	PASS
441	198	0.01	100	14.3	19664	PASS
442	442	50	100	100.0	126659	PASS
443	442	15	24	18.8	23776	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/5/2024	BNA_F	<u>BF136966.D</u>
Compound Name	Response	Retention Time
DDT	307743	13.486
DDD	12060	13.186
DDE	683	12.839
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12743	320486	3.98

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010524\
Data File : BF136966.D
Acq On : 05 Jan 2024 09:45
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 05 11:00:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

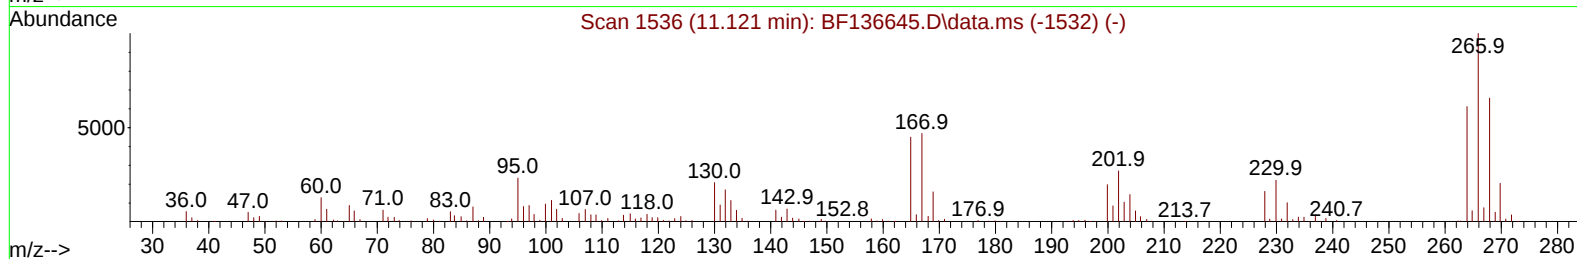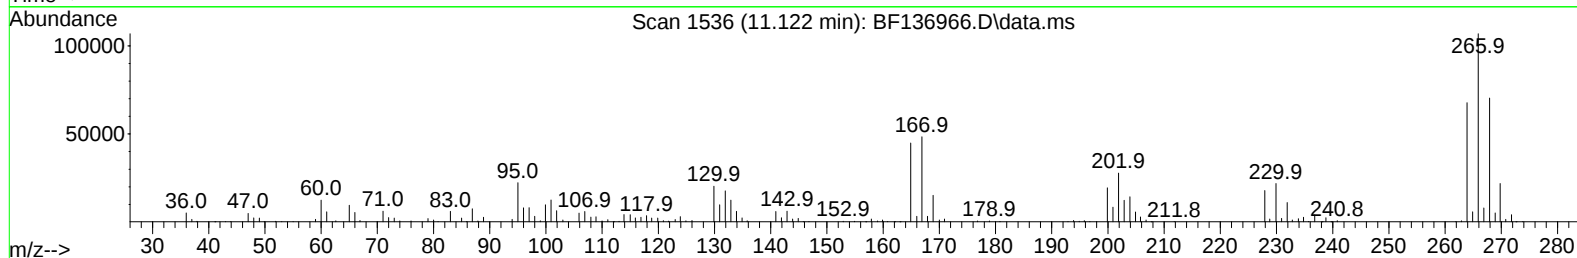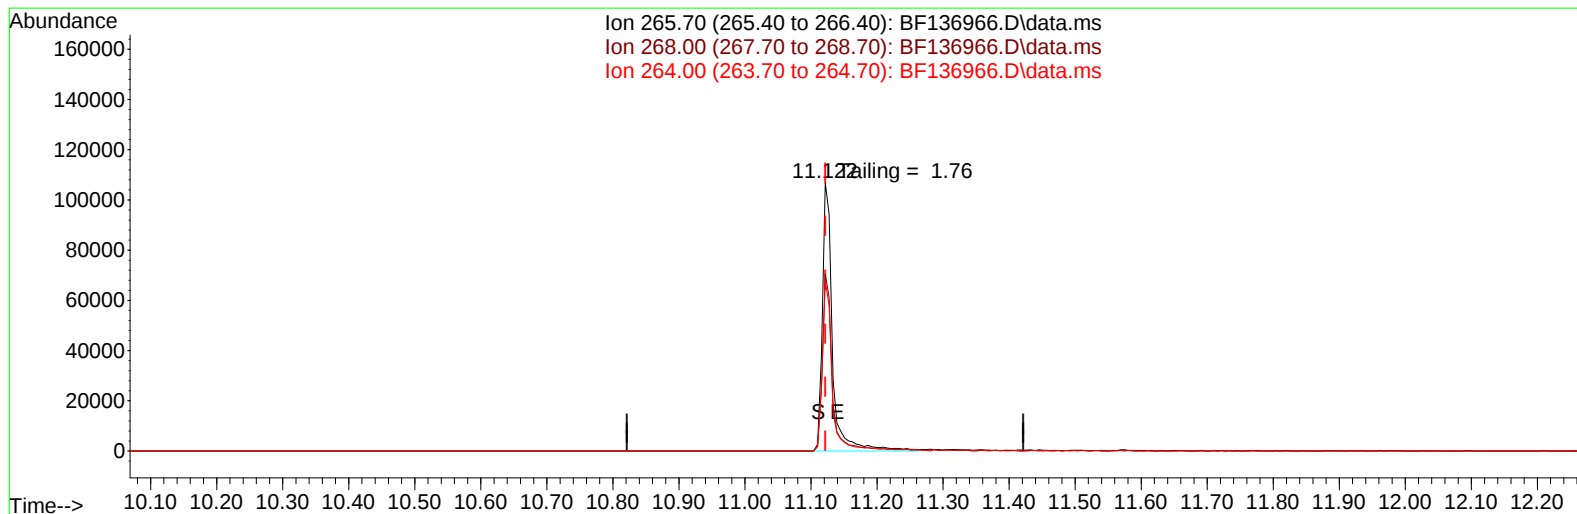

TIC: BF136966.D\data.ms

(70) Pentachlorophenol (C)

11.122min (+ 0.000) 29818.58 ng




response 114563

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	65.87
264.00	61.20	63.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010524\
Data File : BF136966.D
Acq On : 05 Jan 2024 09:45
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 05 11:00:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

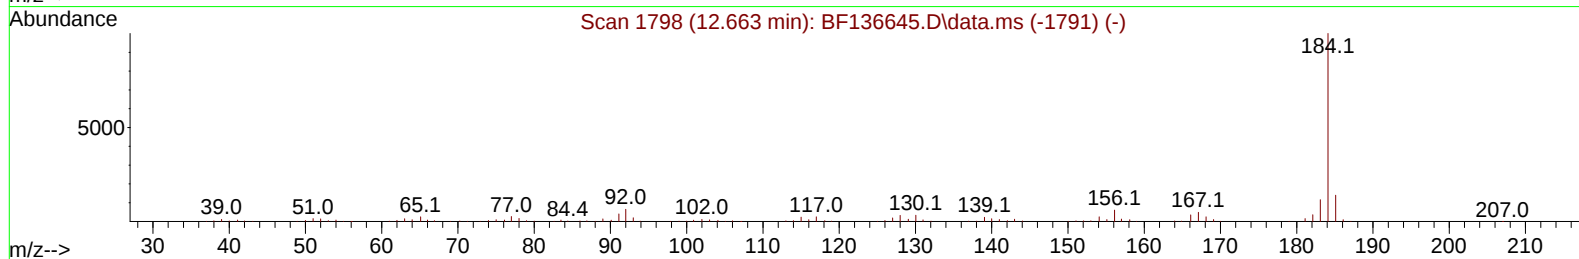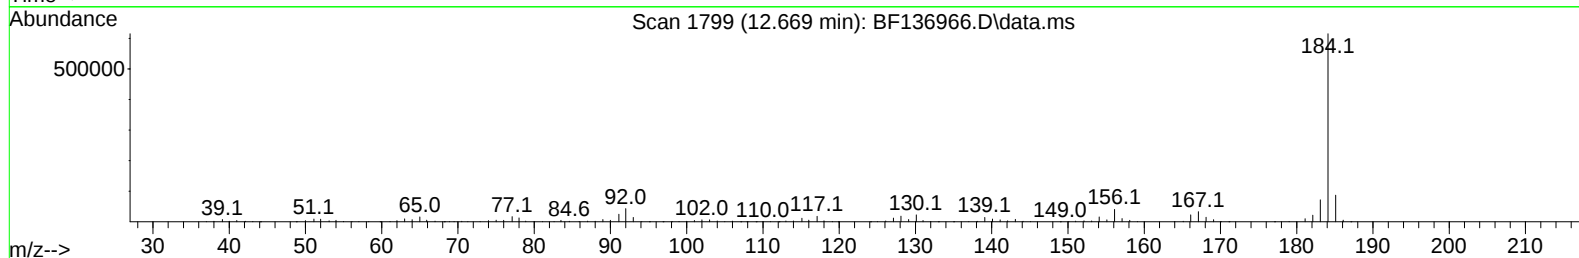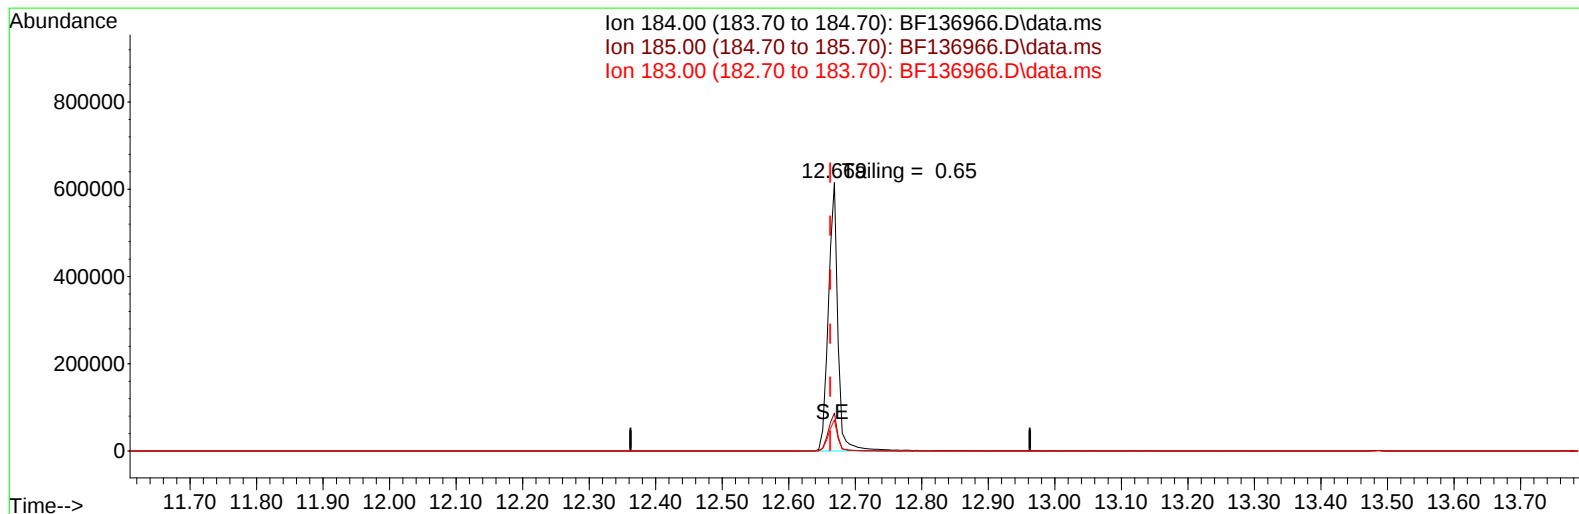

TIC: BF136966.D\data.ms

(77) Benzidine

12.669min (+ 0.006) 320372.05 ng m

response 614016

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.14
183.00	11.60	11.67
0.00	0.00	0.00