
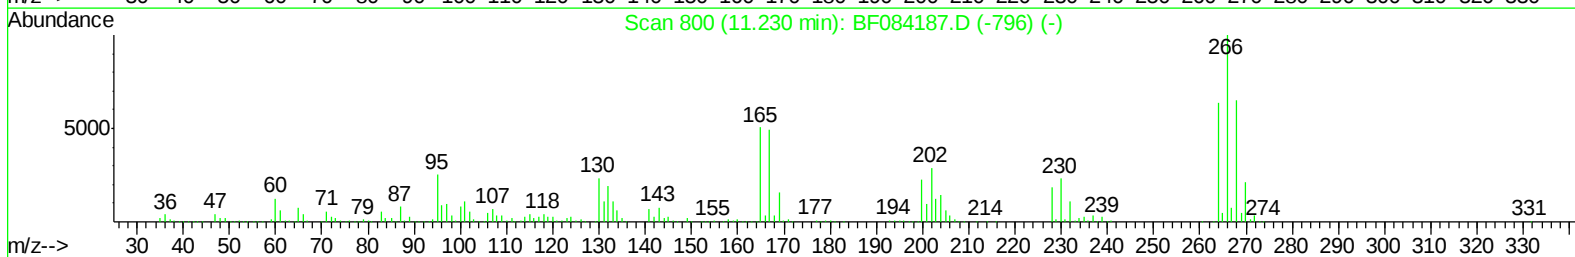
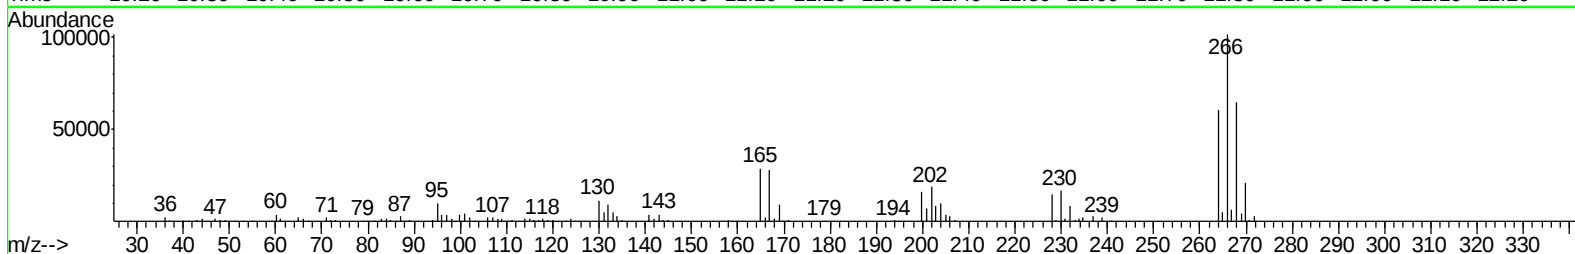


Data Path : Z:\HPCHEM1\BNA F\Data\BF010616\
Data File : BF084279.D
Acq On : 6 Jan 2016 10:20
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 07 04:16:22 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF123115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 04 12:22:40 2016
Response via : Initial Calibration

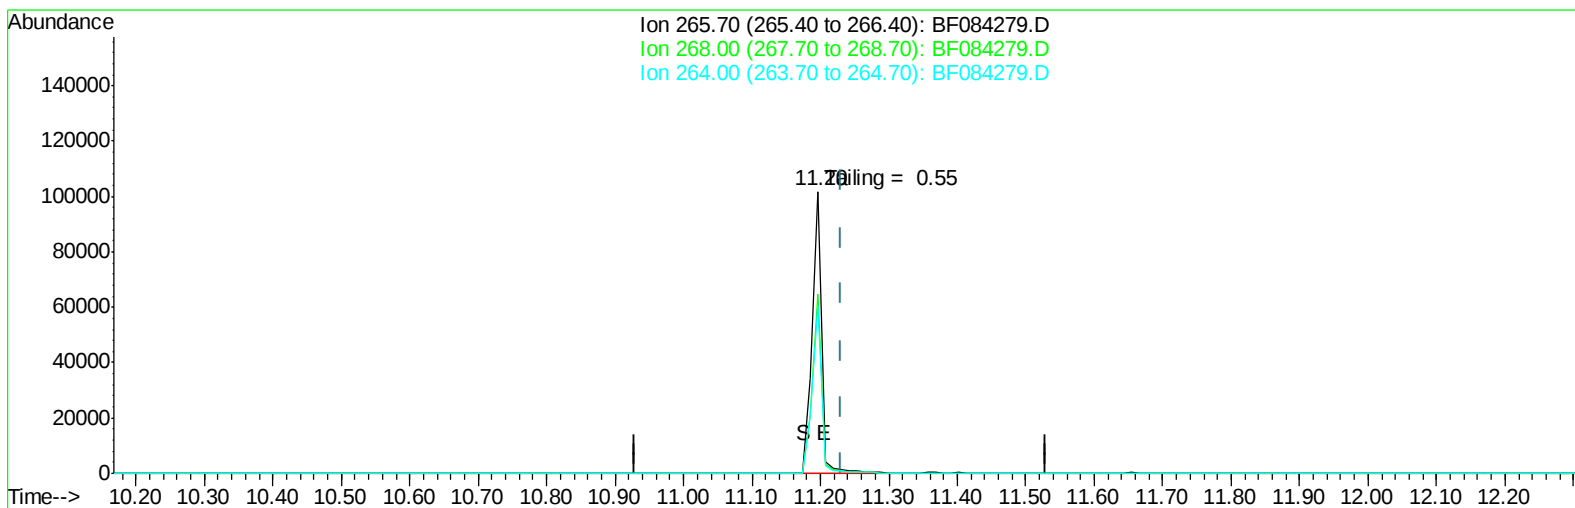

TIC: BF084279.D

(69) Pentachlorophenol (C)




11.196min (-0.034) 14915.15ng

response 100434

Ion	Exp%	Act%
265.70	100	100
268.00	65.50	63.64
264.00	62.70	59.69
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF010616\
 Data File : BF084279.D
 Acq On : 6 Jan 2016 10:20
 Operator : SJ/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 07 04:16:22 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF123115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 04 12:22:40 2016
 Response via : Initial Calibration

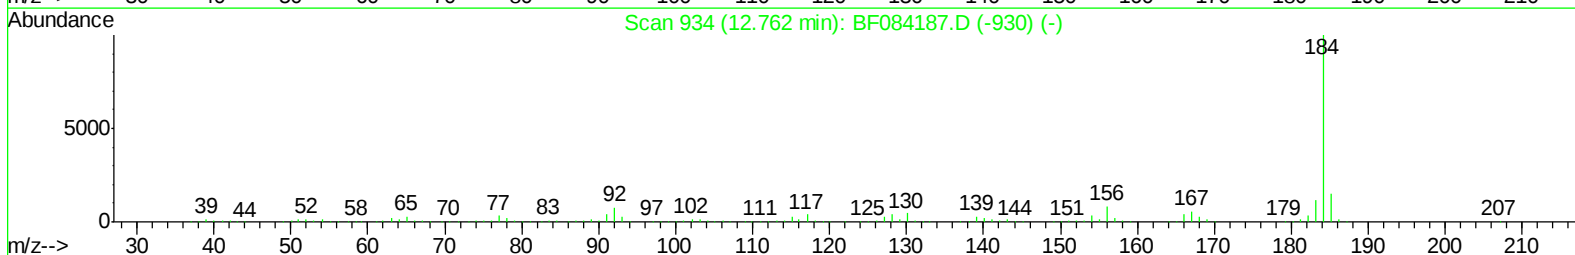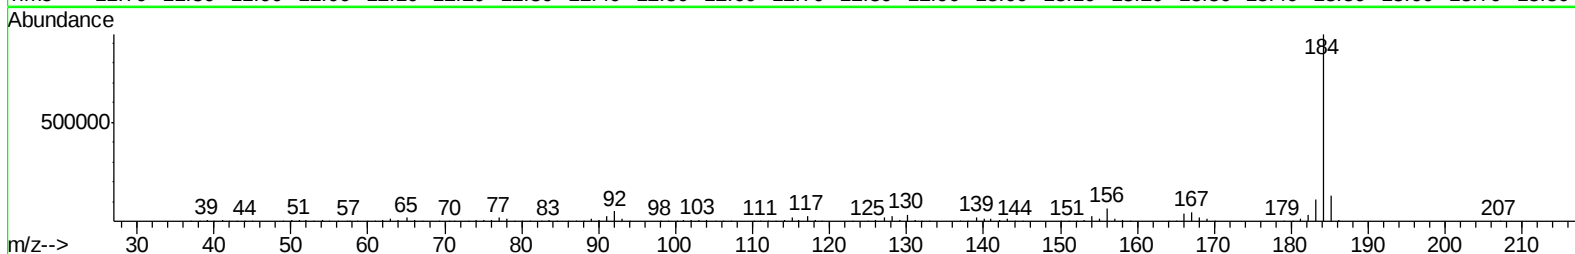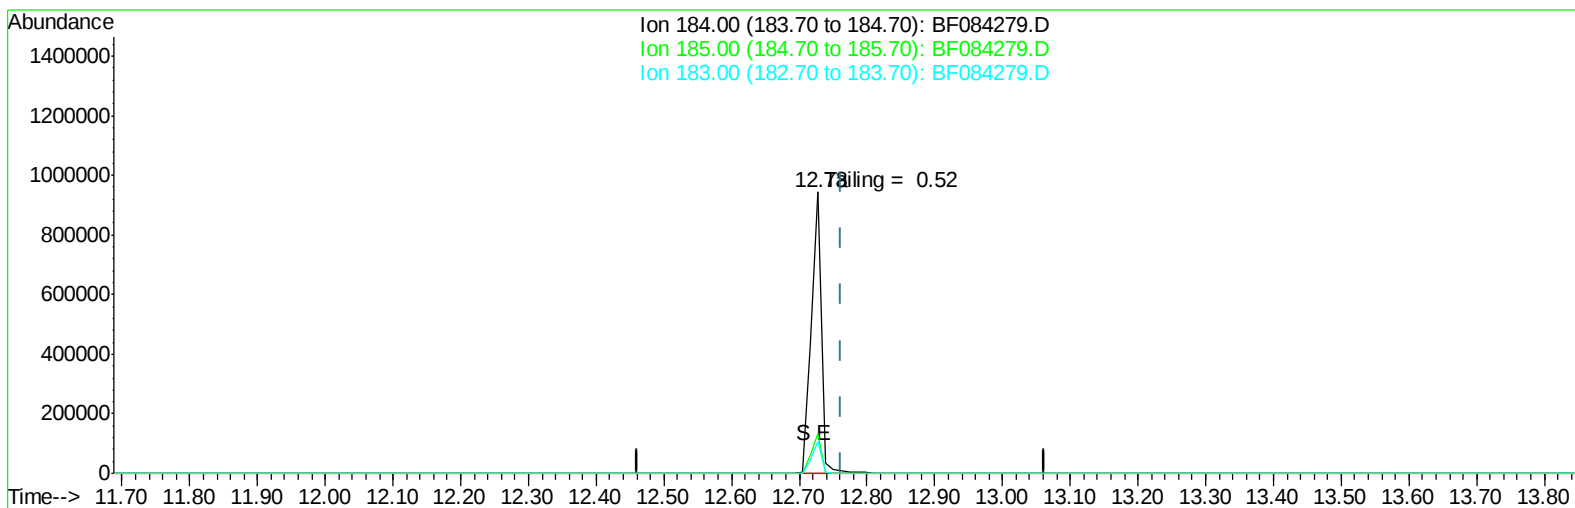

TIC: BF084279.D

(76) Benzidine

12.728min (-0.034) 18886.74ng

response 992076

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.02
183.00	12.30	11.41
0.00	0.00	0.00