


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF010616\
 Data File : BF084279.D
 Acq On : 6 Jan 2016 10:20
 Operator : SJ/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 04 12:22:40 2016

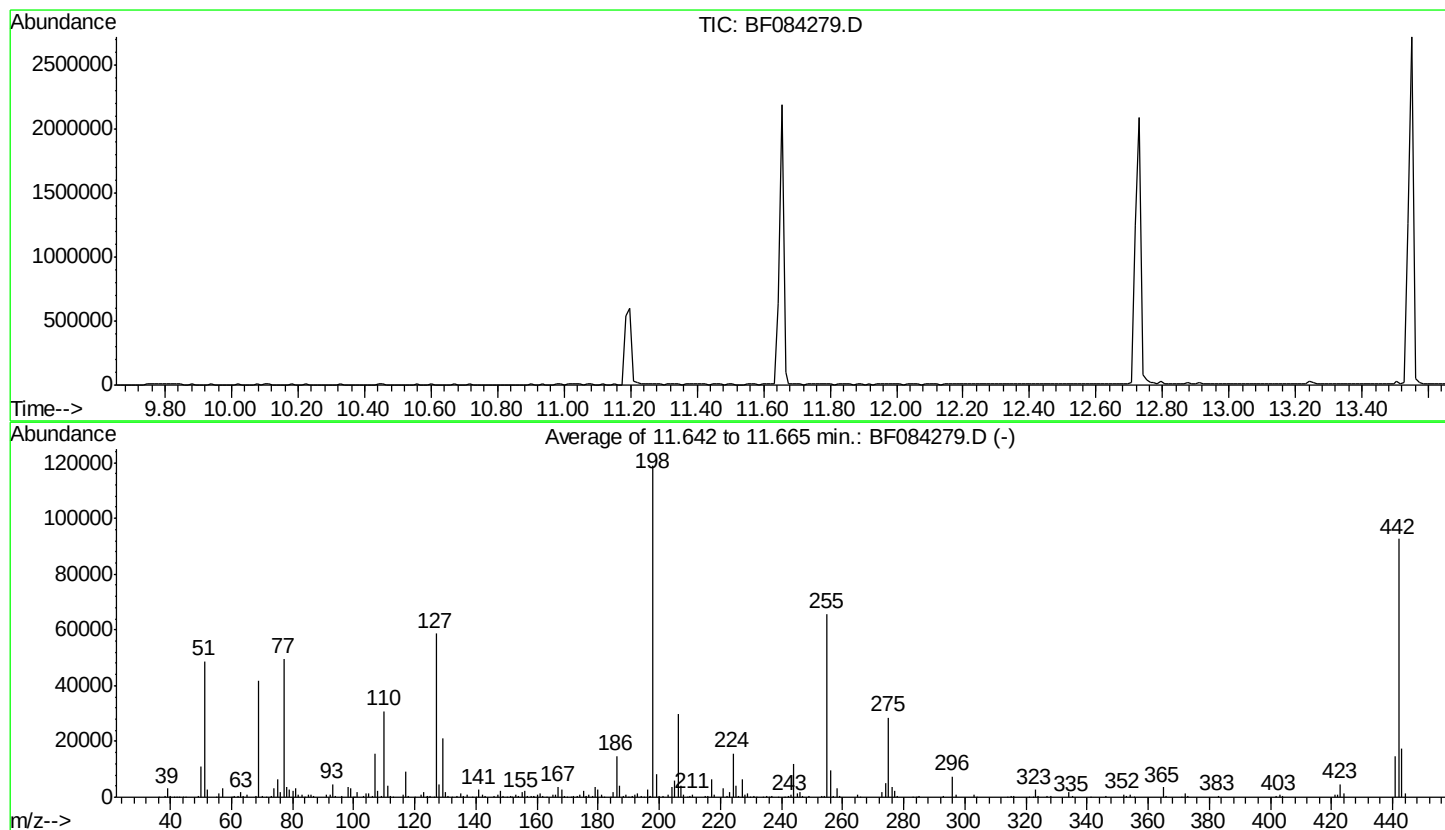

AutoFind: Scans 836, 837, 838; Background Corrected with Scan 833

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.0	48689	PASS
68	69	0.00	2	1.5	638	PASS
69	198	0.00	100	35.1	41731	PASS
70	69	0.00	2	0.8	322	PASS
127	198	10	80	49.3	58633	PASS
197	198	0.00	2	0.5	591	PASS
198	198	100	100	100.0	118884	PASS
199	198	5	9	6.9	8154	PASS
275	198	10	60	24.1	28646	PASS
365	198	1	100	3.1	3647	PASS
441	442	0.01	24	16.0	14803	PASS
442	198	50	100	77.8	92527	PASS
443	442	15	24	18.8	17390	PASS