
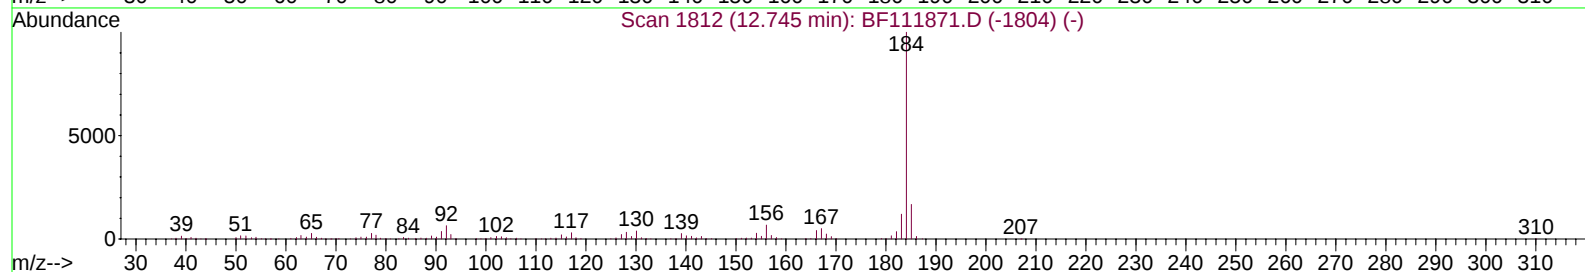
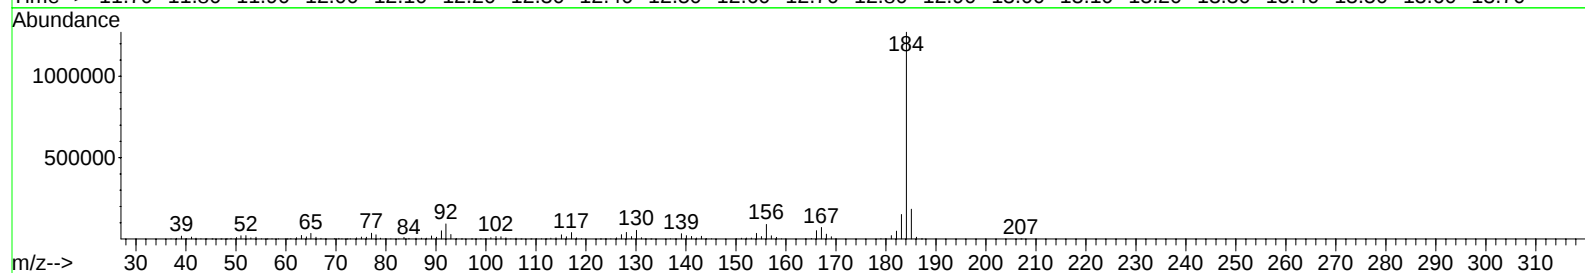


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF010719\
Data File : BF111867.D
Acq On : 7 Jan 2019 10:02
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 07 15:19:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF010719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 07 14:33:51 2019
Response via : Initial Calibration

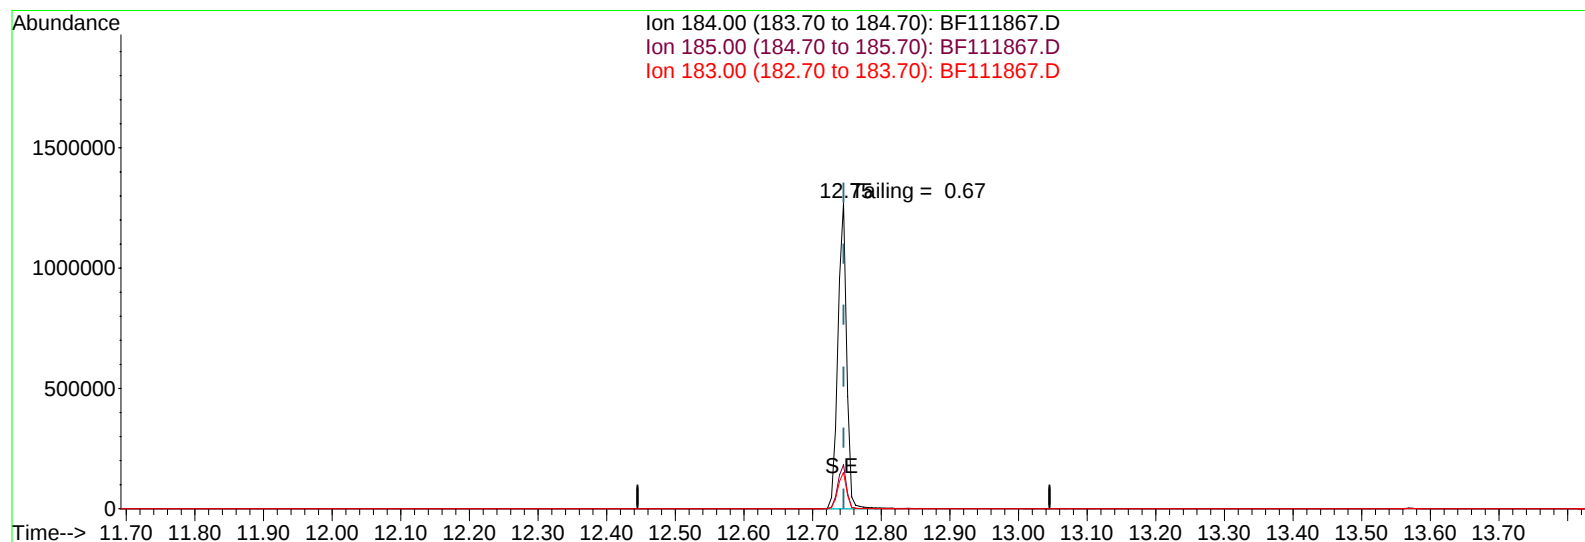

TIC: BF111867.D

(77) Benzidine




12.745min (+0.000) 0.00ng

response 1122546

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.40
183.00	12.00	11.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF010719\
Data File : BF111867.D
Acq On : 7 Jan 2019 10:02
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 07 15:19:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF010719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 07 14:33:51 2019
Response via : Initial Calibration

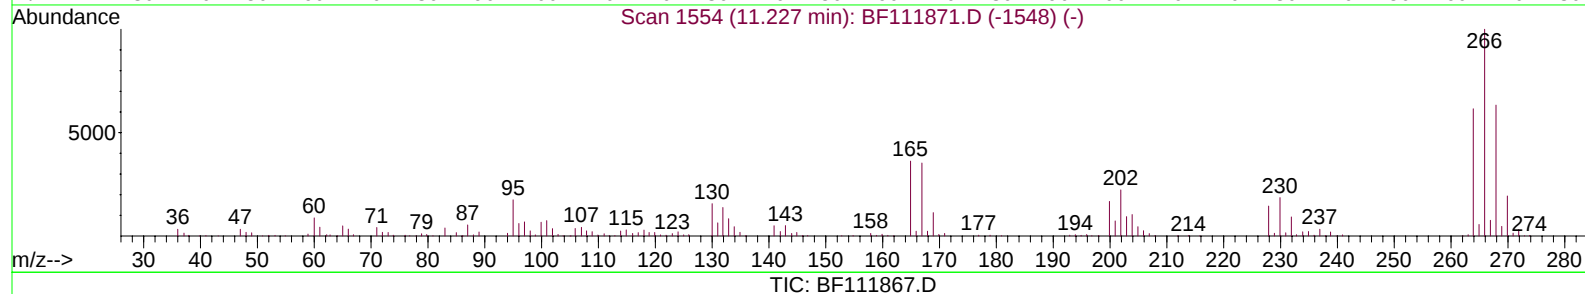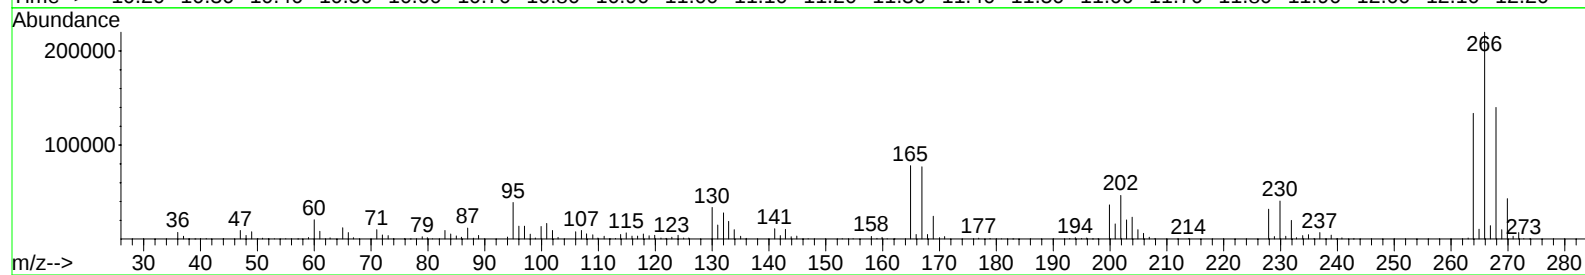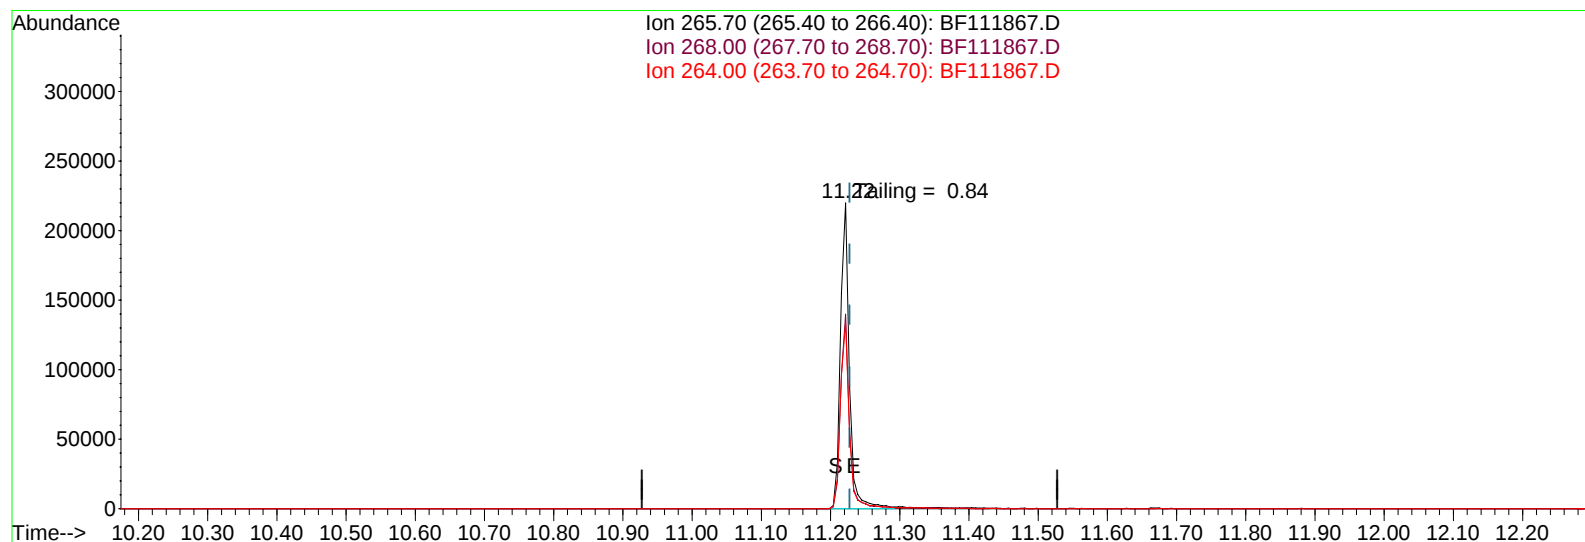

(70) Pentachlorophenol (C)

11.222min (-0.006) 32215.89ng

response 196838

Ion	Exp%	Act%
265.70	100	100
268.00	63.30	63.64
264.00	61.60	60.84
0.00	0.00	0.00