

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF010719\
 Data File : BF111889.D
 Acq On : 7 Jan 2019 21:03
 Operator : JU/SJ
 Sample : K1034-01 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CONTROL-HOUSE-WALL-1-1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF010719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.092	507	511	515	rBV	21518	21677	1.78%	0.259%
2	5.516	580	583	594	rBV	292807	271348	22.24%	3.245%
3	6.528	751	755	767	rBV	275608	286430	23.48%	3.425%
4	6.663	774	778	785	rVB	305031	294149	24.11%	3.517%
5	6.886	812	816	820	rBV	1001664	807662	66.21%	9.658%
6	7.045	839	843	846	rBV	283956	248433	20.37%	2.971%
7	7.439	906	910	921	rBV	201473	181082	14.84%	2.165%
8	8.169	1030	1034	1038	rBV	1156898	984834	80.73%	11.776%
9	8.939	1163	1165	1175	rVB2	14135	21313	1.75%	0.255%
10	9.245	1213	1217	1228	rVB	392114	370688	30.39%	4.433%
11	9.633	1280	1283	1287	rBV	28023	22573	1.85%	0.270%
12	9.927	1329	1333	1340	rBV	1275142	1086897	89.10%	12.997%
13	10.716	1463	1467	1473	rVB	152028	148774	12.20%	1.779%
14	11.410	1582	1585	1589	rBV	1019856	876952	71.89%	10.486%
15	11.933	1669	1674	1677	rBV3	25365	31771	2.60%	0.380%
16	12.833	1821	1827	1828	rBV5	11216	18502	1.52%	0.221%
17	12.992	1850	1854	1863	rVB	403906	350669	28.75%	4.193%
18	13.886	2004	2006	2011	rVB5	33113	41020	3.36%	0.490%
19	14.051	2030	2034	2042	rVB	1191001	1078289	88.39%	12.894%
20	15.533	2281	2286	2293	rBV	932357	1219869	100.00%	14.587%


Sum of corrected areas: 8362932

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF010719\
Data File : BF111889.D
Acq On : 7 Jan 2019 21:03
Operator : JU/SJ
Sample : K1034-01 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CONTROL-HOUSE-WALL-1-1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF010719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

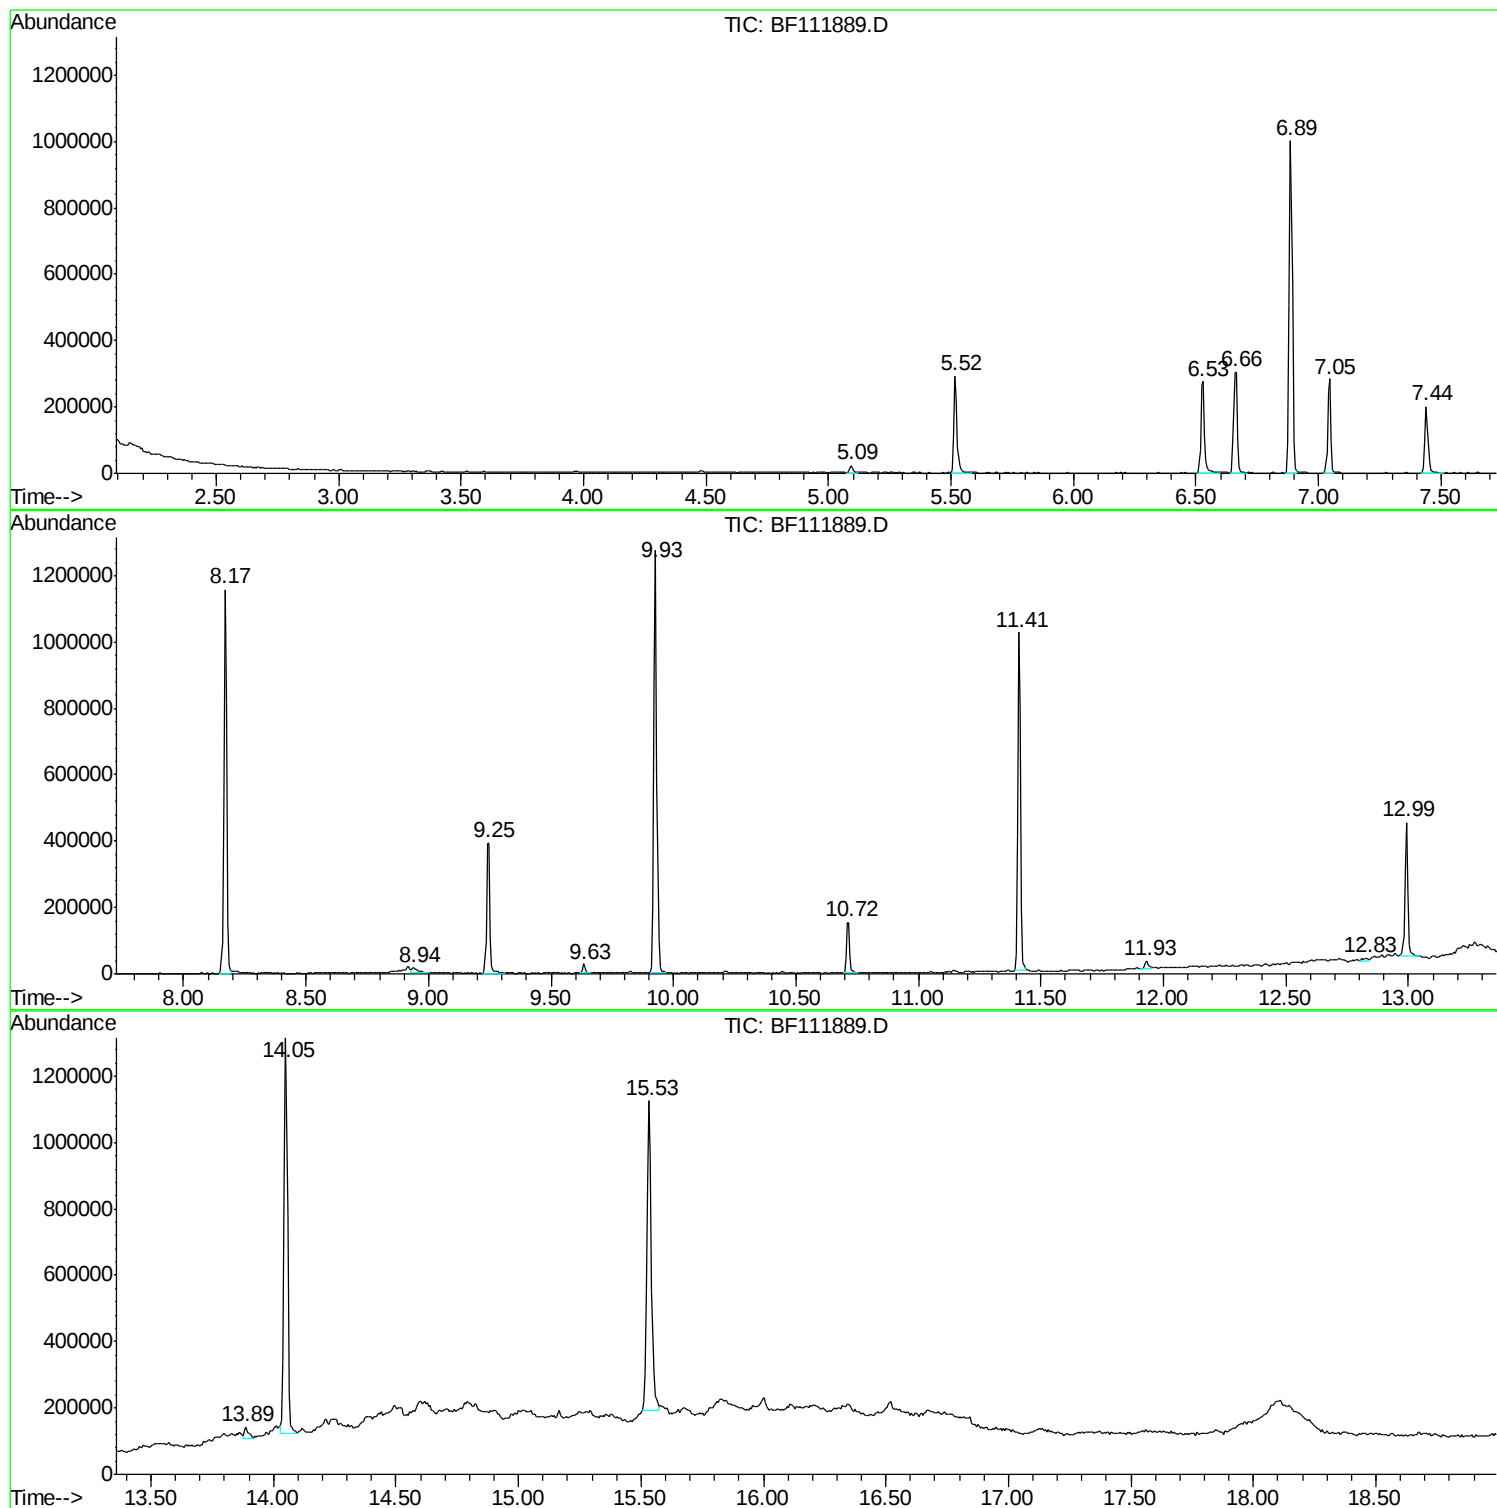

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF010719\
Data_File : BF111889.D
Acq_On : 7 Jan 2019 21:033
Operator : JU/SJJ
Sample : K1034-01_10XX
Misc :
ALS_Vial : 13 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
CONTROL-HOUSE-WALL-1-1

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF010719.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
