

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF010719\
 Data File : BF111890.D
 Acq On : 7 Jan 2019 21:30
 Operator : JU/SJ
 Sample : K1034-02 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CONTROL-HOUSE-WALL-1-2

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF010719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.092	507	511	517	rBV	26730	26978	2.36%	0.387%
2	5.516	580	583	589	rBV	209832	200530	17.52%	2.880%
3	6.528	751	755	765	rBV	214932	216780	18.94%	3.113%
4	6.663	774	778	786	rVB	269664	249597	21.81%	3.584%
5	6.886	812	816	820	rBV	1032967	842745	73.65%	12.102%
6	7.045	839	843	846	rBV	271617	233649	20.42%	3.355%
7	7.439	907	910	917	rBV	182883	161049	14.07%	2.313%
8	8.169	1030	1034	1042	rBV	1038996	846972	74.02%	12.163%
9	9.239	1213	1216	1225	rBV	269942	252371	22.05%	3.624%
10	9.927	1329	1333	1338	rBV	915435	797888	69.73%	11.458%
11	10.710	1463	1466	1474	rVB	99450	91734	8.02%	1.317%
12	11.410	1582	1585	1589	rBV	827605	702565	61.40%	10.089%
13	12.992	1850	1854	1857	rBV	239640	204467	17.87%	2.936%
14	13.898	2003	2008	2011	rBV7	11476	21764	1.90%	0.313%
15	14.051	2030	2034	2038	rBV	996903	865238	75.61%	12.425%
16	14.209	2059	2061	2063	rBV3	13488	12268	1.07%	0.176%
17	14.257	2066	2069	2070	rBV3	14749	18334	1.60%	0.263%
18	14.374	2085	2089	2090	rBV2	27597	34665	3.03%	0.498%
19	14.827	2164	2166	2168	rBV3	20485	18104	1.58%	0.260%
20	15.168	2222	2224	2227	rBV	24077	21601	1.89%	0.310%
21	15.533	2281	2286	2296	rVB	883344	1144289	100.00%	16.432%


Sum of corrected areas: 6963588

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF010719\
Data File : BF111890.D
Acq On : 7 Jan 2019 21:30
Operator : JU/SJ
Sample : K1034-02 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CONTROL-HOUSE-WALL-1-2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF010719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

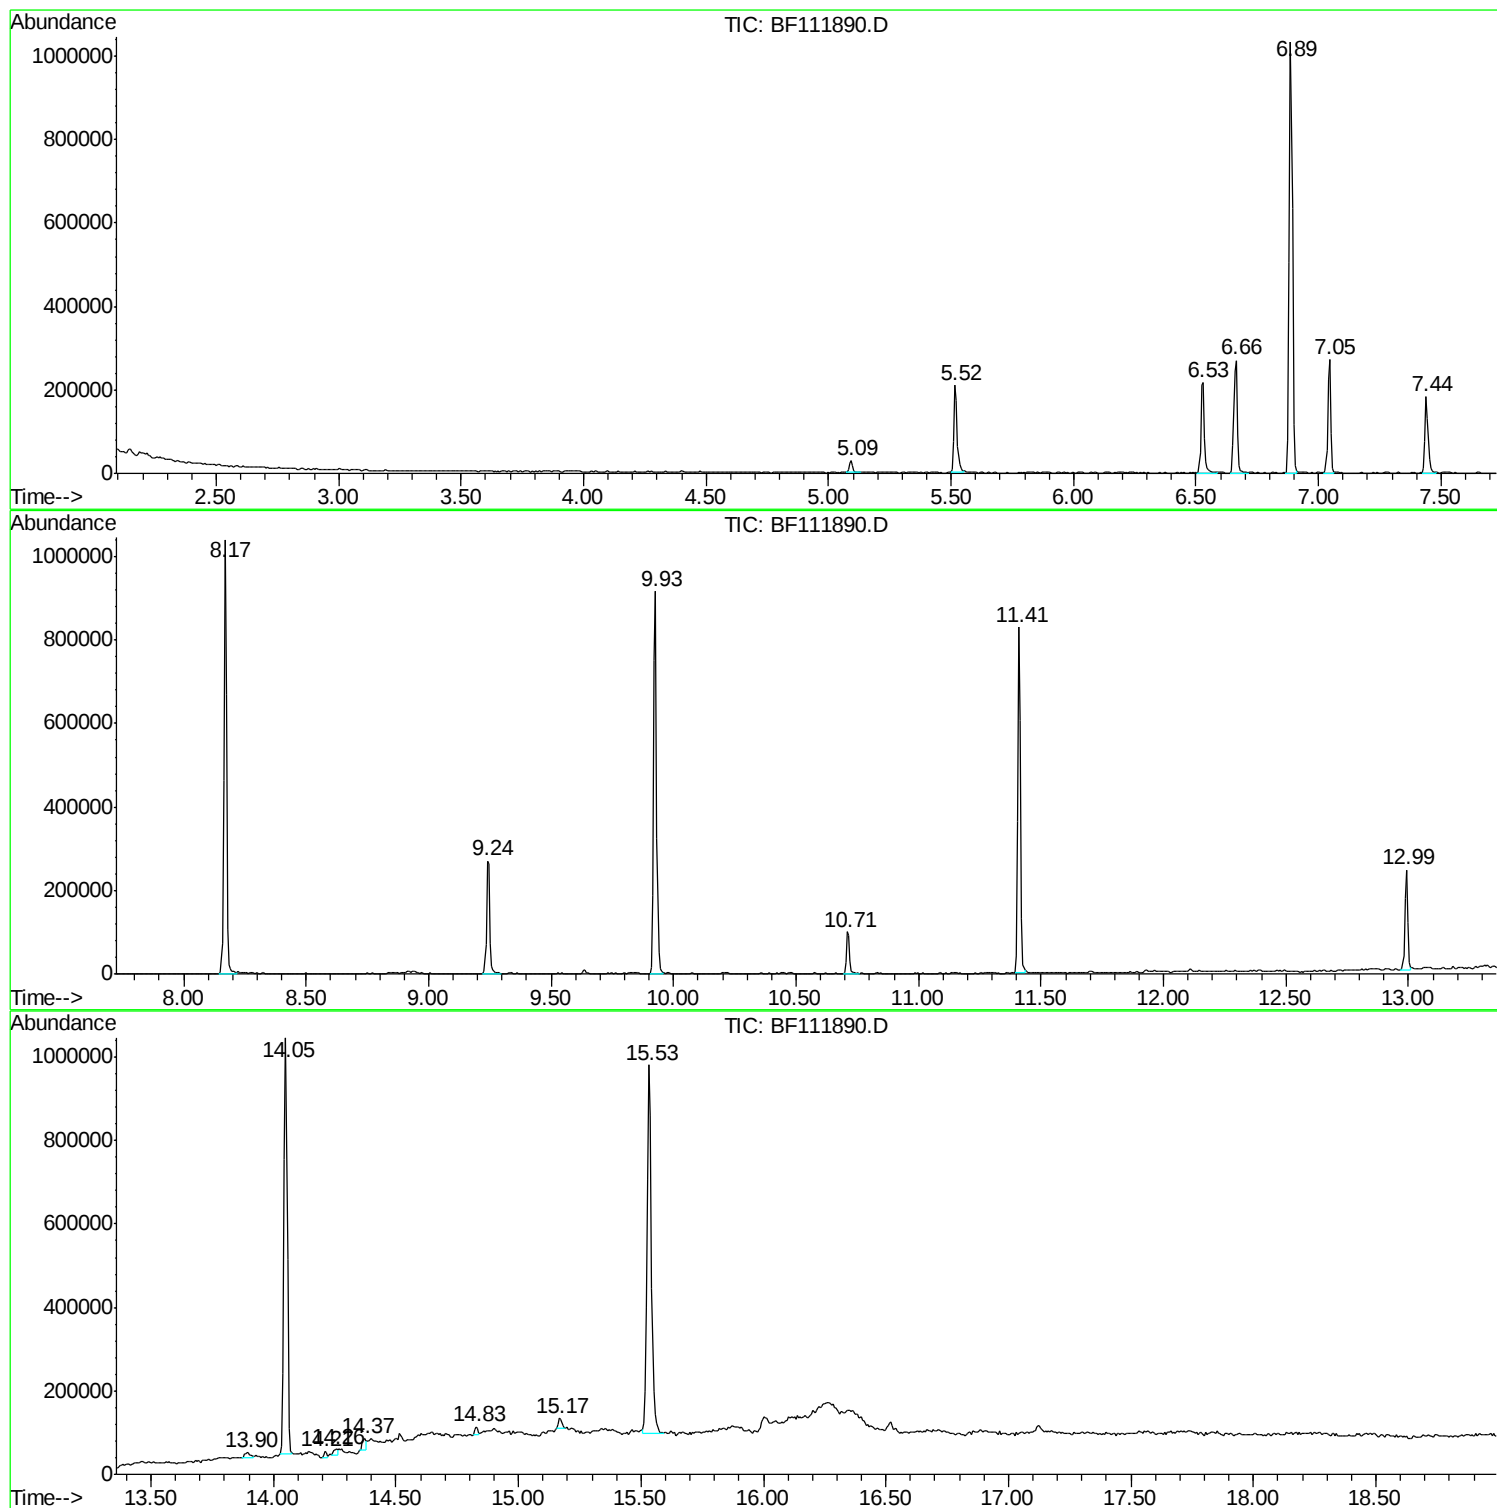

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF010719\
Data File : BF111890.D
Acq On : 7 Jan 2019 21:30
Operator : JU/SJ
Sample : K1034-02 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CONTROL-HOUSE-WALL-1-2










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF010719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.66 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.66	5.92 ng	249597	1,4-Dichlorobenzene-d4	6.89

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2			1H-Indazole, 7-methyl-	132	C8H8N2	1000316-00-7	25
3			5-Aminoindole	132	C8H8N2	005192-03-0	22
4			(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
5			N-(3,4-Methylenedioxyphenyl)isop...	267	C17H17NO2	1000378-96-6	10

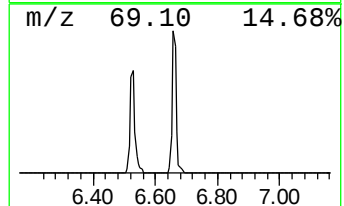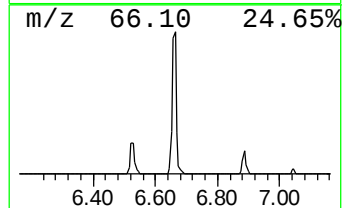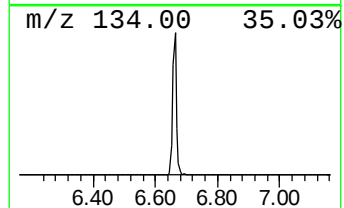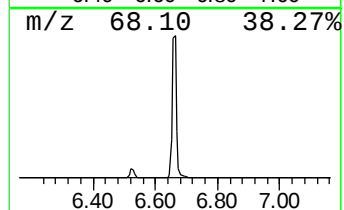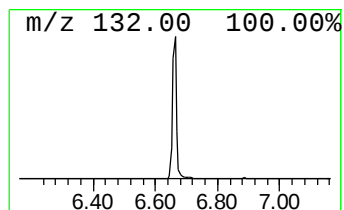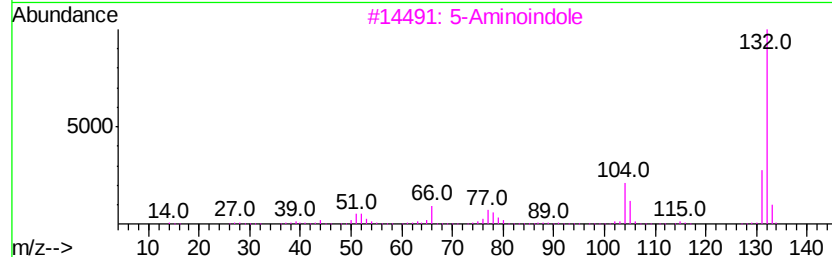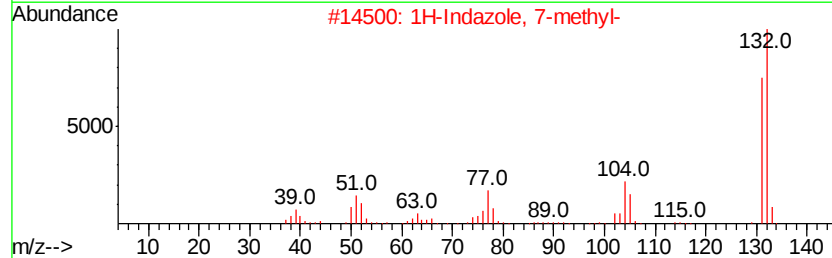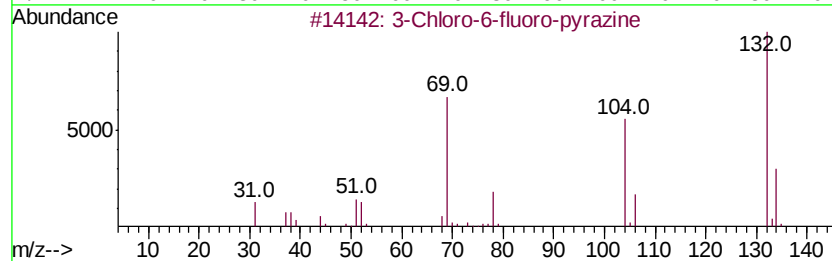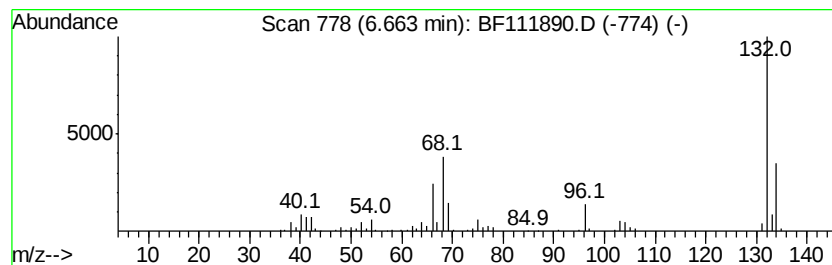

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF010719\
Data File : BF111890.D
Acq On : 7 Jan 2019 21:30
Operator : JU/SJ
Sample : K1034-02 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CONTROL-HOUSE-WALL-1-2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF010719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.66	6.66	5.9	ng	249597	1	6.89	842745	20.0