

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF010719\
 Data File : BF111891.D
 Acq On : 7 Jan 2019 21:58
 Operator : JU/SJ
 Sample : K1034-03 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CONTROL-HOUSE-WALL-1-3

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF010719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.516	580	583	594	rBV	174421	179476	17.13%	2.558%
2	6.528	751	755	762	rBV	190622	195349	18.64%	2.784%
3	6.663	774	778	782	rBV	215086	194765	18.59%	2.776%
4	6.886	812	816	820	rBV	1058349	870785	83.11%	12.410%
5	7.045	839	843	846	rBV	202871	167309	15.97%	2.384%
6	7.439	907	910	918	rBV	128150	115978	11.07%	1.653%
7	8.169	1030	1034	1038	rBV	1212014	1001839	95.62%	14.277%
8	9.245	1213	1217	1226	rBV	203375	185854	17.74%	2.649%
9	9.633	1279	1283	1288	rVB	17294	17053	1.63%	0.243%
10	9.927	1329	1333	1340	rVB	1063360	898688	85.77%	12.807%
11	10.716	1464	1467	1471	rBV	75807	71778	6.85%	1.023%
12	11.410	1582	1585	1589	rBV	801298	702706	67.07%	10.014%
13	12.992	1850	1854	1857	rBV	226729	178328	17.02%	2.541%
14	13.886	2003	2006	2013	rBV5	20956	35128	3.35%	0.501%
15	14.051	2030	2034	2043	rVB	1117806	971514	92.73%	13.845%
16	14.515	2111	2113	2117	rBV2	17336	18001	1.72%	0.257%
17	14.827	2164	2166	2170	rVB3	21777	17053	1.63%	0.243%
18	14.980	2188	2192	2193	rBV4	14438	17942	1.71%	0.256%
19	15.162	2221	2223	2227	rVB3	27850	31659	3.02%	0.451%
20	15.392	2260	2262	2263	rBV2	13564	12592	1.20%	0.179%
21	15.533	2281	2286	2294	rBV	827205	1047735	100.00%	14.931%
22	15.998	2363	2365	2370	rVB2	25576	32537	3.11%	0.464%
23	16.209	2396	2401	2402	rBV5	34258	52957	5.05%	0.755%


Sum of corrected areas: 7017026

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF010719\
Data File : BF111891.D
Acq On : 7 Jan 2019 21:58
Operator : JU/SJ
Sample : K1034-03 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CONTROL-HOUSE-WALL-1-3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF010719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

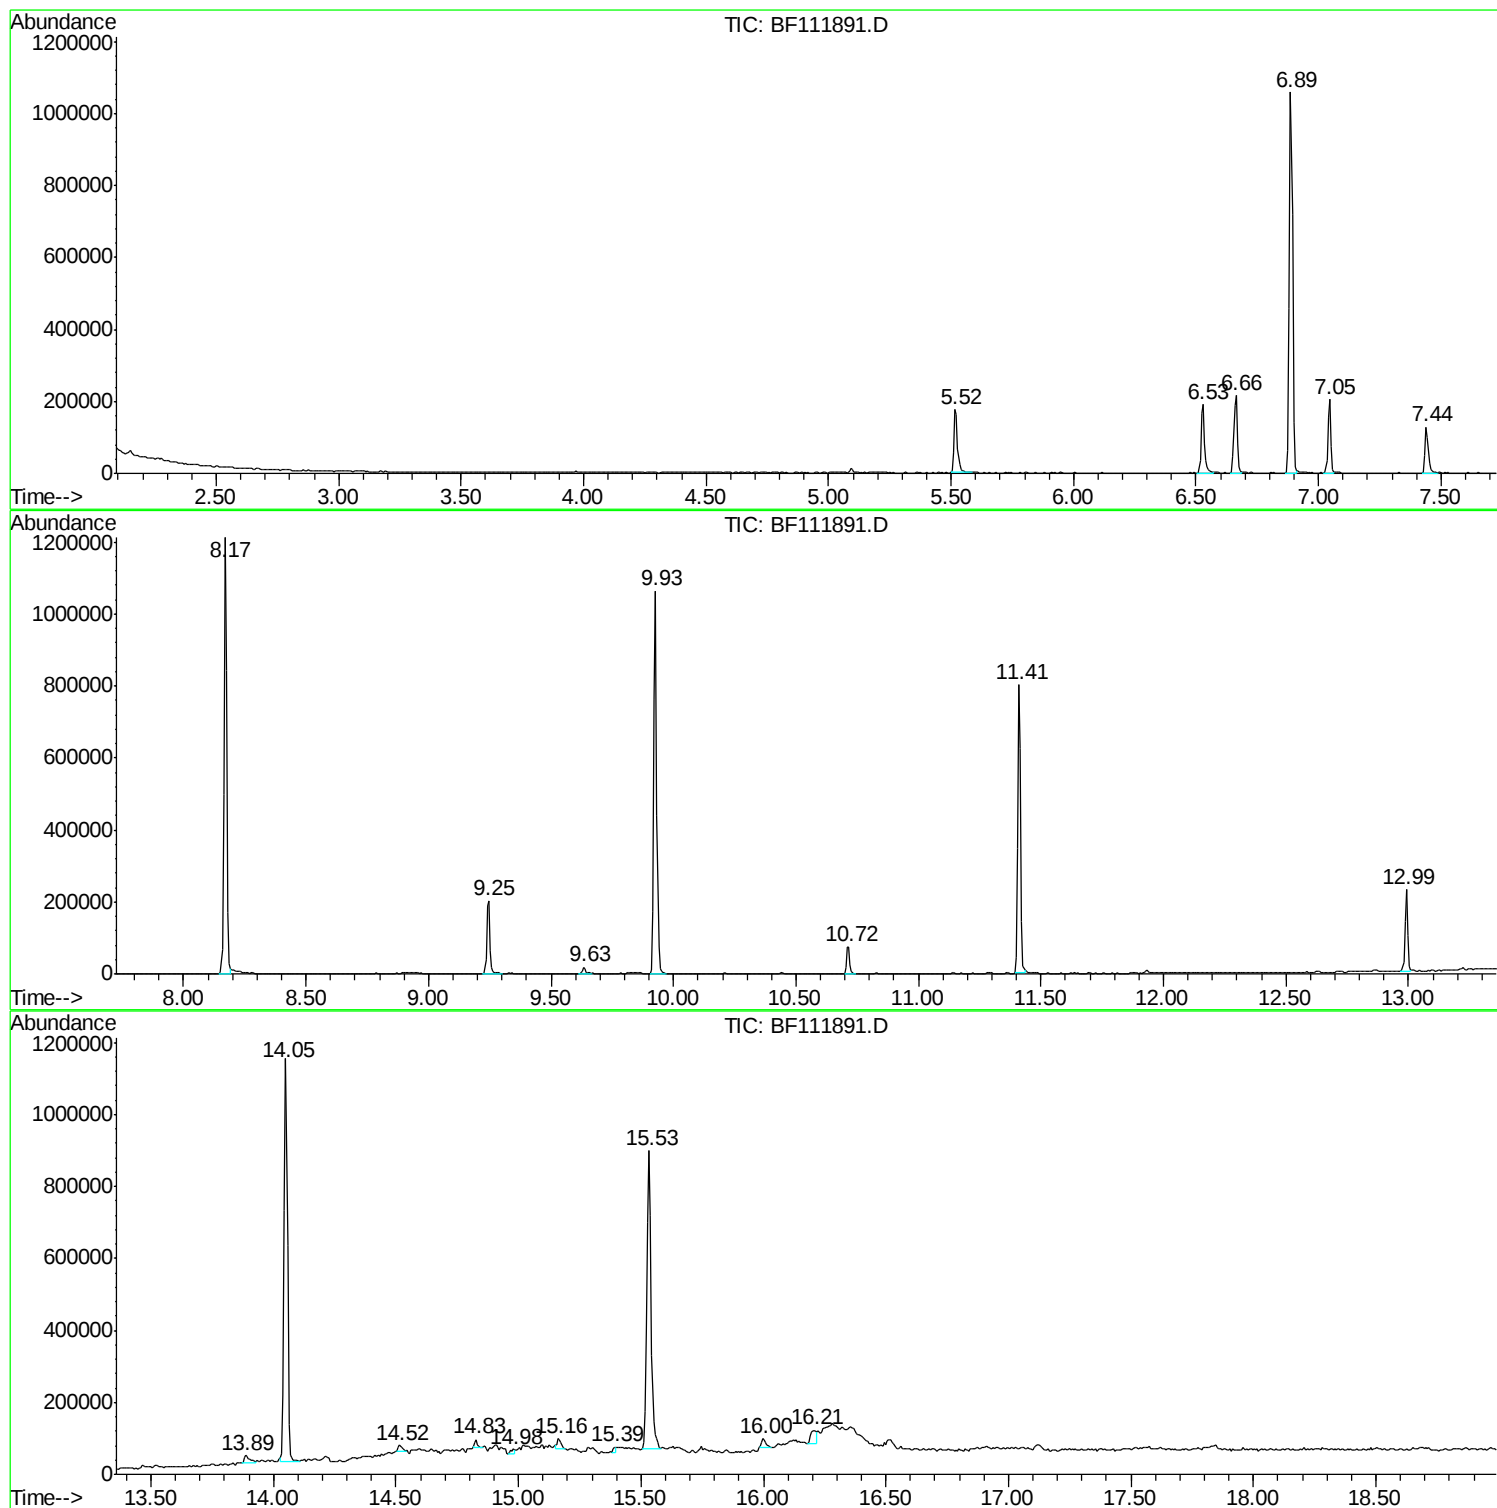

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF010719\
Data File : BF111891.D
Acq On : 7 Jan 2019 21:58
Operator : JU/SJ
Sample : K1034-03 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CONTROL-HOUSE-WALL-1-3










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF010719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.66 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.66	4.47 ng	194765	1,4-Dichlorobenzene-d4	6.89

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	25
2		Tranvlcypromine-propionyl	189	C12H15NO	1000123-86-3	16
3		Benzene, 1-ethenyl-3,5-dimethyl-	132	C10H12	005379-20-4	9
4		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9
5		1-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-59-9	9

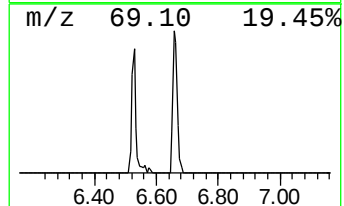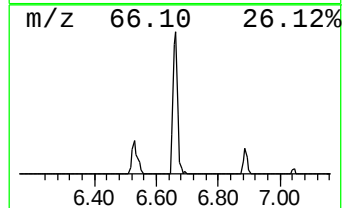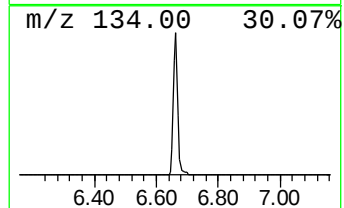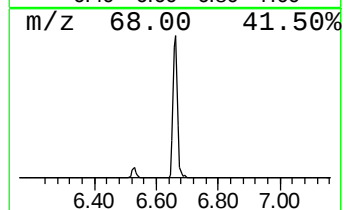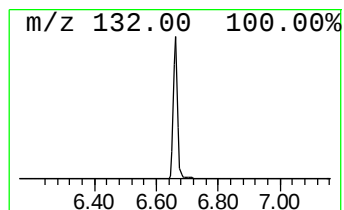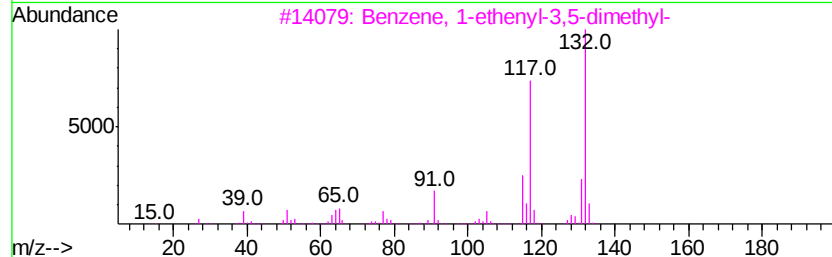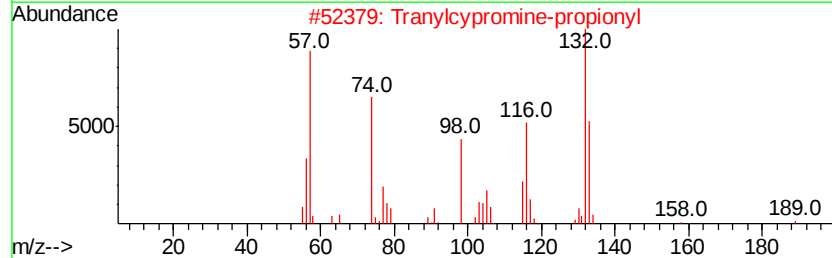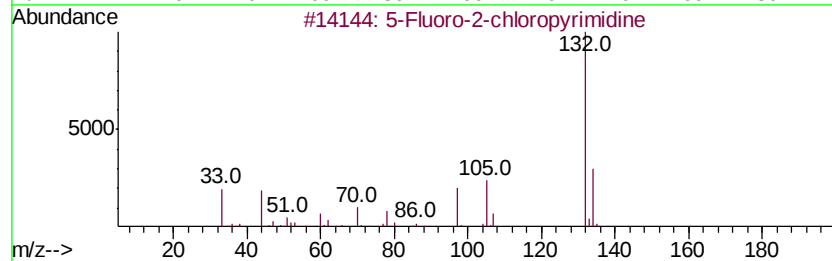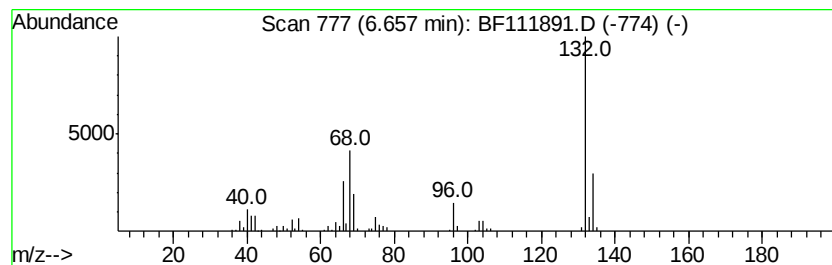

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF010719\
Data File : BF111891.D
Acq On : 7 Jan 2019 21:58
Operator : JU/SJ
Sample : K1034-03 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CONTROL-HOUSE-WALL-1-3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF010719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.66	6.66	4.5	ng	194765	1	6.89	870785	20.0