

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF010719\
 Data File : BF111892.D
 Acq On : 7 Jan 2019 22:25
 Operator : JU/SJ
 Sample : K1034-04 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CONTROL-HOUSE-WALL-1-4

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF010719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.093	507	511	518	rBV	35652	35594	3.32%	0.462%
2	5.516	580	583	590	rBV	194172	194234	18.10%	2.521%
3	6.522	751	754	768	rBV	260471	254782	23.74%	3.307%
4	6.657	774	777	785	rBV	245588	232582	21.67%	3.019%
5	6.887	812	816	820	rBV	1147744	900603	83.90%	11.689%
6	7.045	839	843	846	rBV	280545	244080	22.74%	3.168%
7	7.439	907	910	917	rBV	196353	167963	15.65%	2.180%
8	8.169	1030	1034	1038	rBV	1339450	1070573	99.74%	13.895%
9	9.245	1213	1217	1225	rBV	318326	295296	27.51%	3.833%
10	9.928	1329	1333	1337	rBV	1094410	973421	90.69%	12.634%
11	10.710	1464	1466	1471	rBV	86654	80068	7.46%	1.039%
12	11.410	1581	1585	1589	rBV	968160	822532	76.63%	10.676%
13	12.992	1850	1854	1857	rBV	305908	257756	24.01%	3.345%
14	13.892	2004	2007	2010	rBV3	14389	17789	1.66%	0.231%
15	14.051	2030	2034	2037	rBV	1096596	977869	91.10%	12.692%
16	14.515	2110	2113	2115	rBV2	16843	15031	1.40%	0.195%
17	14.827	2163	2166	2169	rBV4	23523	22791	2.12%	0.296%
18	15.168	2221	2224	2229	rVB2	29967	29252	2.73%	0.380%
19	15.533	2280	2286	2295	rVB	860114	1073399	100.00%	13.932%
20	15.998	2363	2365	2370	rVB3	29590	39167	3.65%	0.508%


Sum of corrected areas: 7704782

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF010719\
Data File : BF111892.D
Acq On : 7 Jan 2019 22:25
Operator : JU/SJ
Sample : K1034-04 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CONTROL-HOUSE-WALL-1-4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF010719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

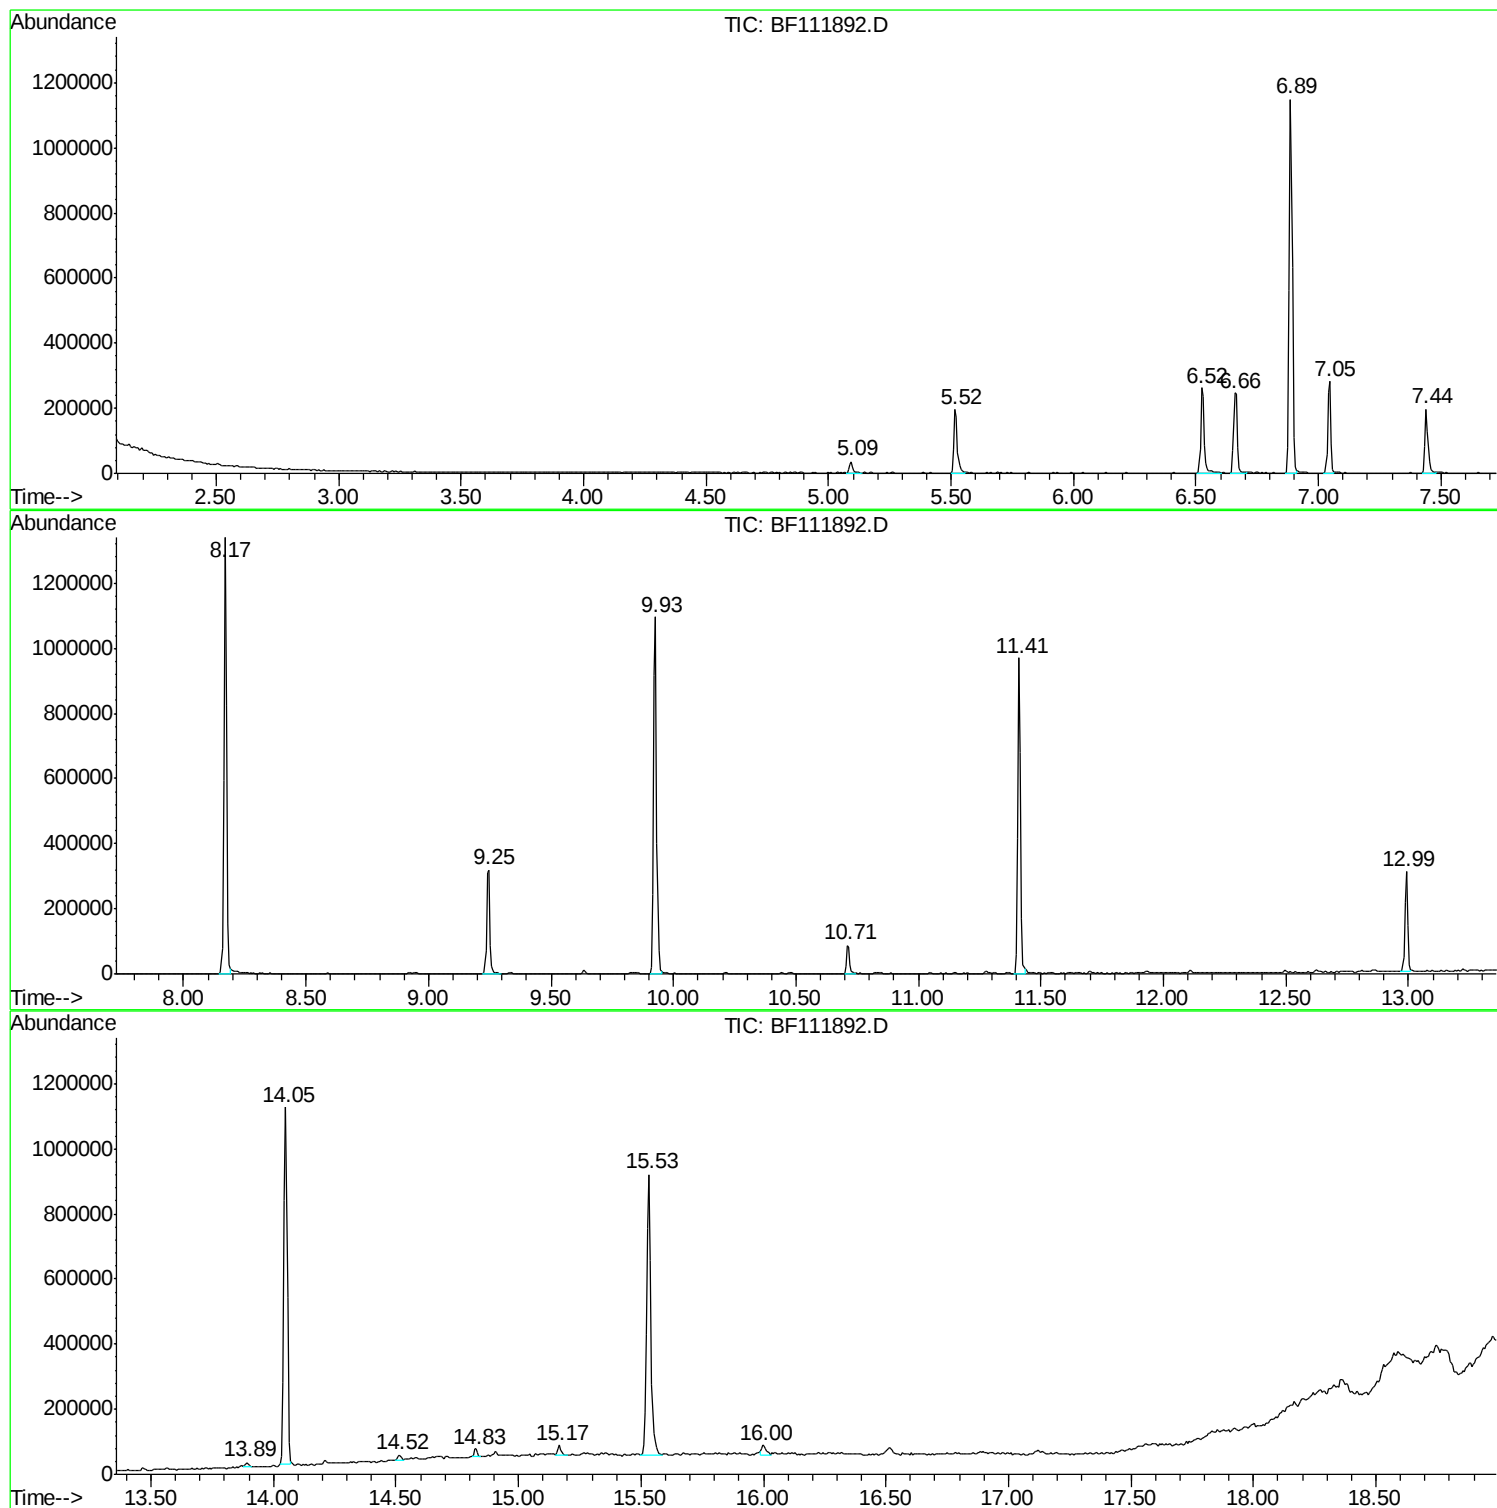

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF010719\
Data File : BF111892.D
Acq On : 7 Jan 2019 22:25
Operator : JU/SJ
Sample : K1034-04 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CONTROL-HOUSE-WALL-1-4










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF010719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.66 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.66	5.17 ng	232582	1,4-Dichlorobenzene-d4	6.89

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	5-Fluoro-2-chloropvrimidine	132	C4H2ClFN2	062802-42-0	12		
2	5-Aminoindole	132	C8H8N2	005192-03-0	10		
3	Xenon	132	Xe	007440-63-3	9		
4	Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9		
5	Benzene, 1-ethenyl-3,5-dimethyl-	132	C10H12	005379-20-4	9		

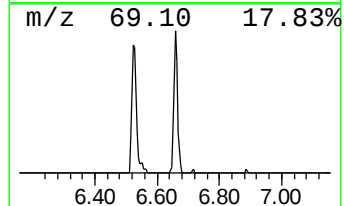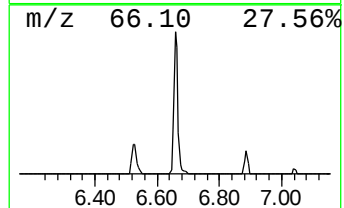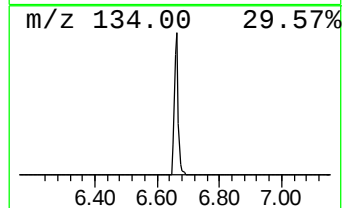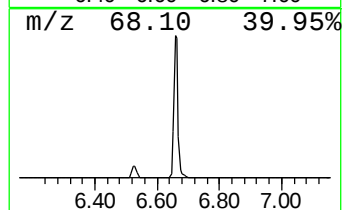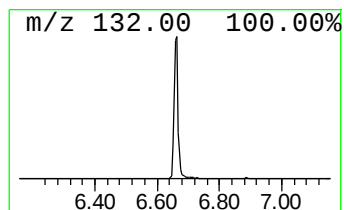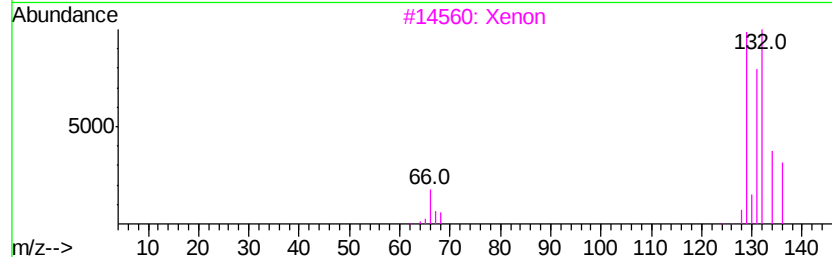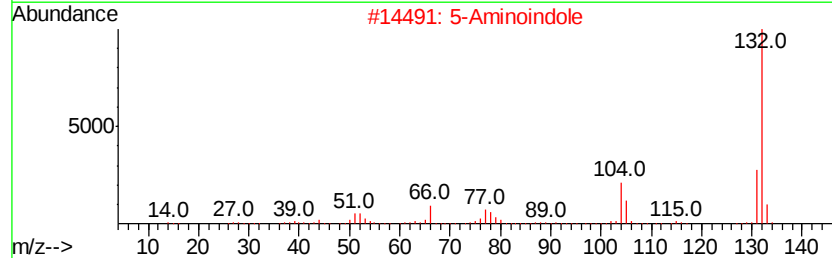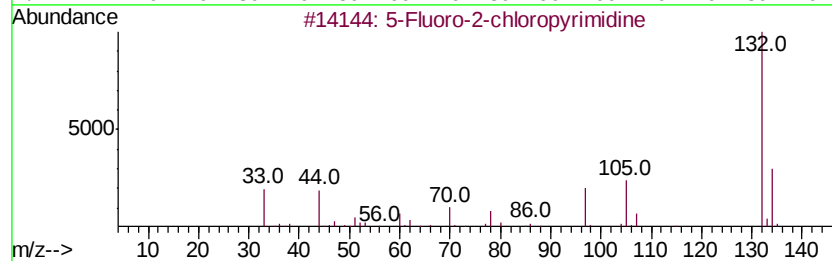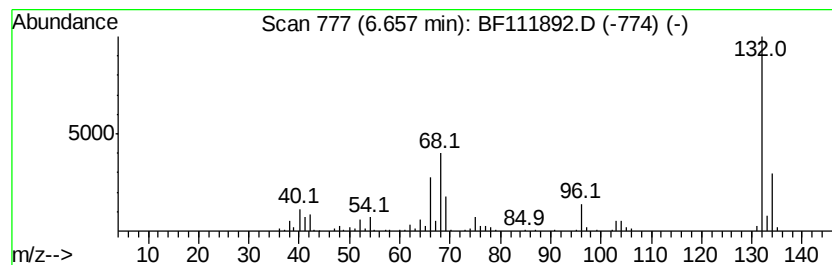

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF010719\
Data File : BF111892.D
Acq On : 7 Jan 2019 22:25
Operator : JU/SJ
Sample : K1034-04 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CONTROL-HOUSE-WALL-1-4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF010719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.66	6.66	5.2	ng	232582	1	6.89	900603	20.0