


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010719\
 Data File : BF111867.D
 Acq On : 7 Jan 2019 10:02
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF010719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 07 14:33:51 2019

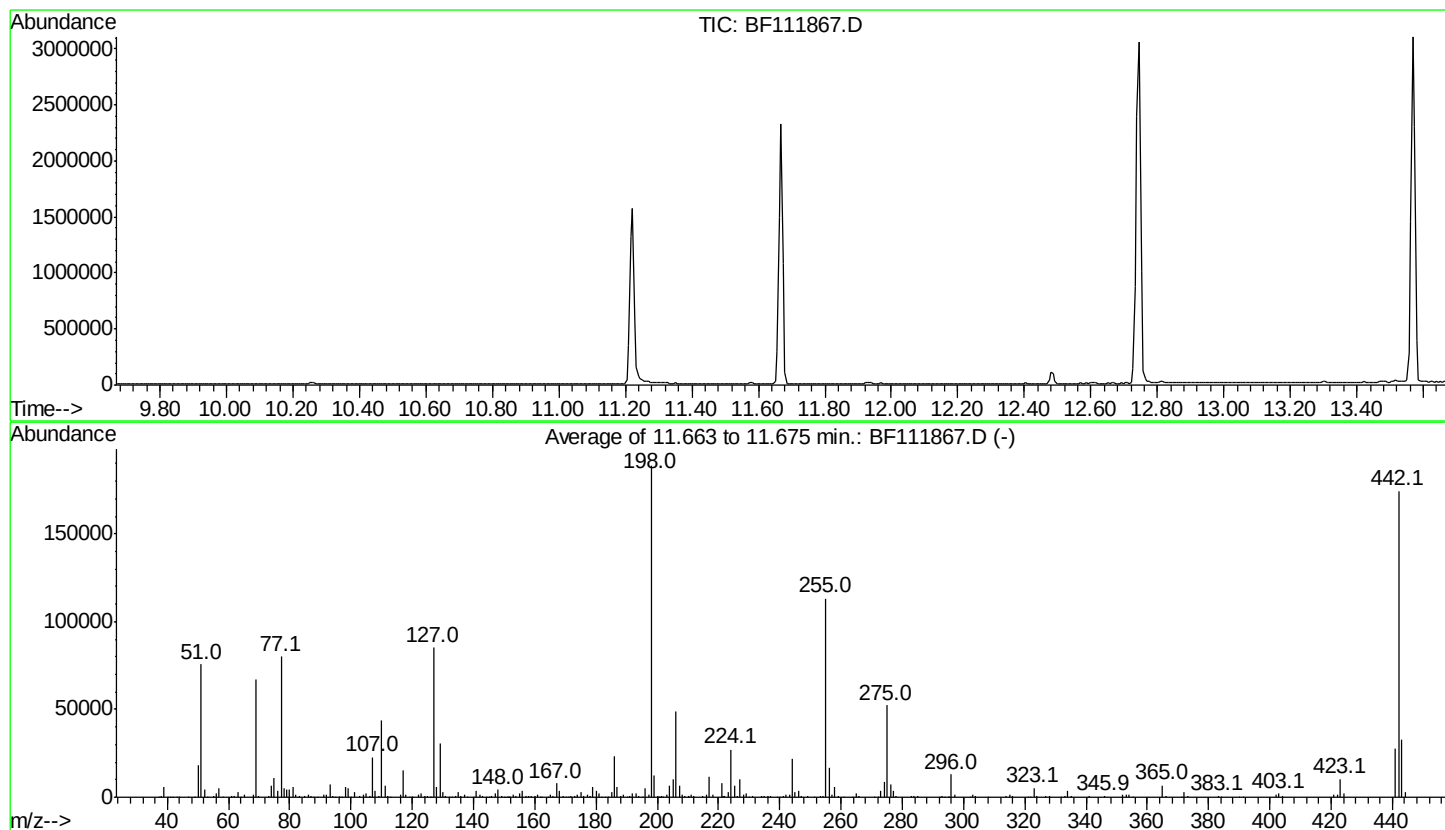

AutoFind: Scans 1628, 1629, 1630; Background Corrected with Scan 1623

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.0	75625	PASS
68	69	0.00	2	1.9	1253	PASS
69	198	0.00	100	35.5	67082	PASS
70	69	0.00	2	0.7	460	PASS
127	198	10	80	45.0	84976	PASS
197	198	0.00	2	0.6	1207	PASS
198	198	100	100	100.0	188904	PASS
199	198	5	9	6.5	12321	PASS
275	198	10	60	27.7	52330	PASS
365	198	1	100	3.7	6910	PASS
441	198	0.01	100	14.6	27584	PASS
442	198	50	100	92.4	174493	PASS
443	442	15	24	18.7	32592	PASS