


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010721\
 Data File : BF122925.D
 Acq On : 7 Jan 2021 15:11
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF010721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 08 01:05:04 2021

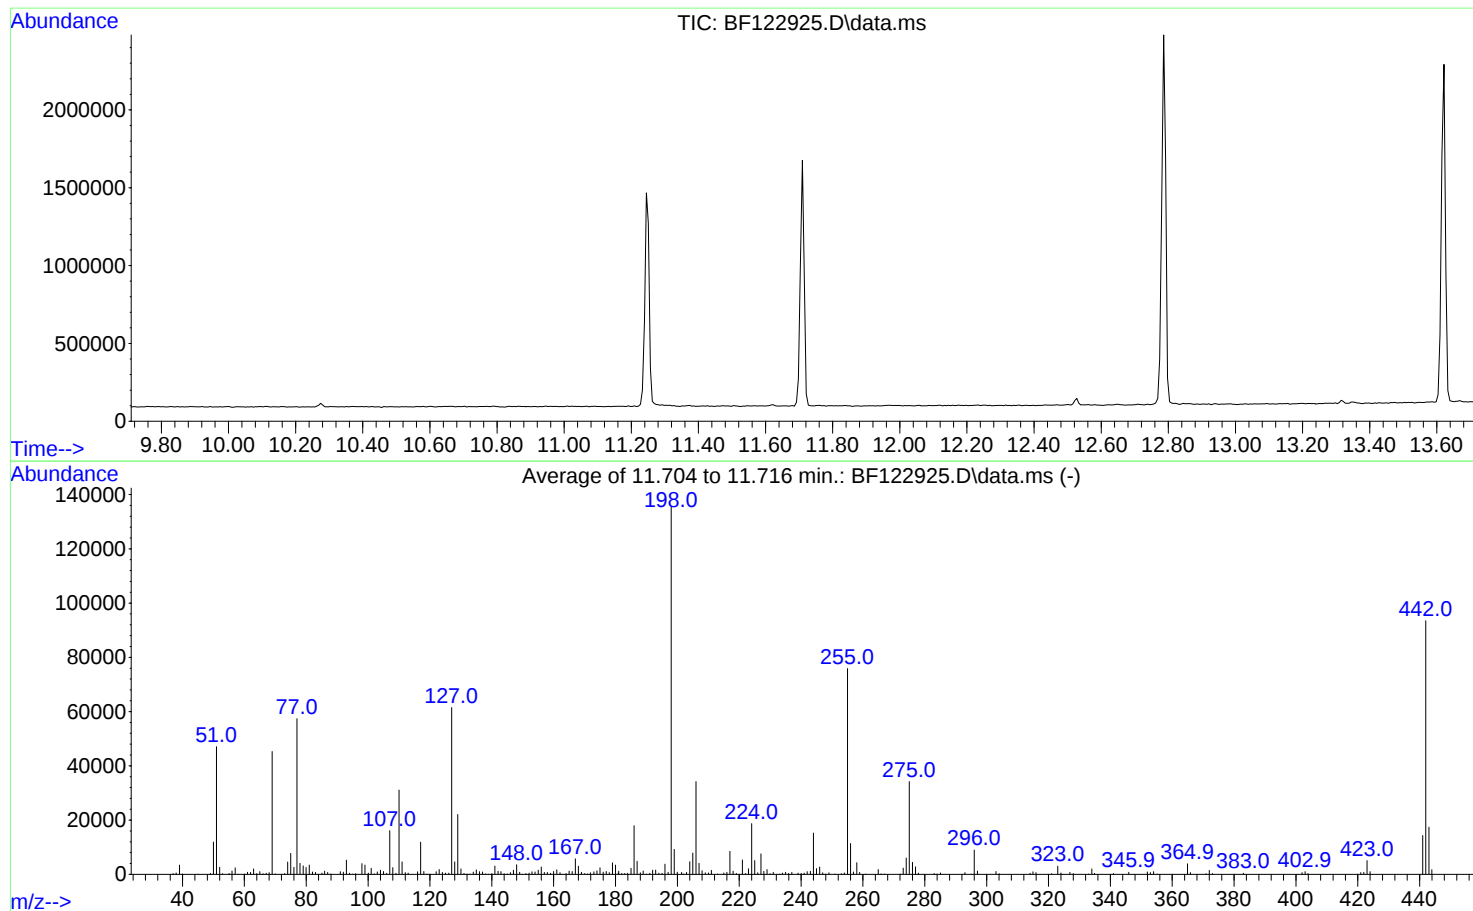

AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.7	47101	PASS
68	69	0.00	2	1.4	632	PASS
69	198	0.00	100	33.4	45329	PASS
70	69	0.00	2	0.4	165	PASS
127	198	10	80	45.3	61464	PASS
197	198	0.00	2	0.6	767	PASS
198	198	100	100	100.0	135608	PASS
199	198	5	9	6.8	9178	PASS
275	198	10	60	25.2	34237	PASS
365	198	1	100	2.9	3923	PASS
441	198	0.01	100	10.6	14339	PASS
442	442	100	100	100.0	93509	PASS
443	442	15	24	18.6	17376	PASS